



US 20030199907A1

(19) **United States**

(12) **Patent Application Publication**

Boecker et al.

(10) **Pub. No.: US 2003/0199907 A1**

(43) **Pub. Date: Oct. 23, 2003**

(54) **METHOD AND APPARATUS FOR  
PENETRATING TISSUE**

(75) Inventors: **Dirk Boecker**, Palo Alto, CA (US);  
**Don Alden**, Sunnyvale, CA (US);  
**Dominique M. Freeman**, La Honda,  
CA (US)

Correspondence Address:  
**HELLER EHRMAN WHITE & MCAULIFFE  
LLP**  
**275 MIDDLEFIELD ROAD**  
**MENLO PARK, CA 94025-3506 (US)**

(73) Assignee: **Pelikan Technologies, Inc.**, Palo Alto,  
CA

(21) Appl. No.: **10/335,240**

(22) Filed: **Dec. 31, 2002**

**Related U.S. Application Data**


(63) Continuation-in-part of application No. 10/127,395,  
filed on Apr. 19, 2002.

**Publication Classification**

(51) **Int. Cl.<sup>7</sup>** ..... **A61B 17/14; A61B 17/32**  
(52) **U.S. Cl.** ..... **606/181; 604/117**

(57) **ABSTRACT**

A tissue penetration device includes a penetrating member driver and a cartridge. A plurality of penetrating members are integrated with the cartridge. Each penetrating member is coupled to the penetrating member driver when advanced along a path into a tissue target. A penetrating member sensor is coupled to the plurality of penetrating members. The penetrating member sensor is configured to provide information relative to a depth of penetration of a penetrating member through a skin surface.

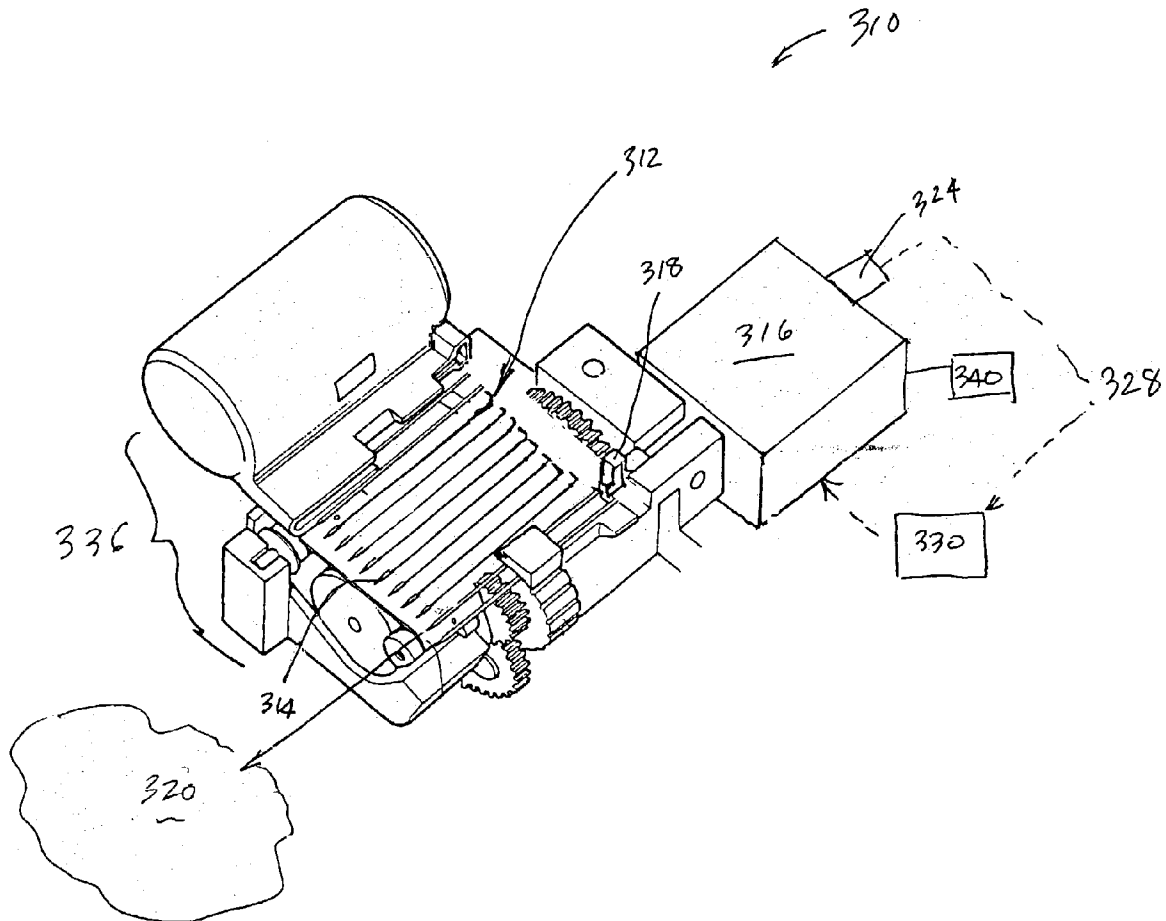

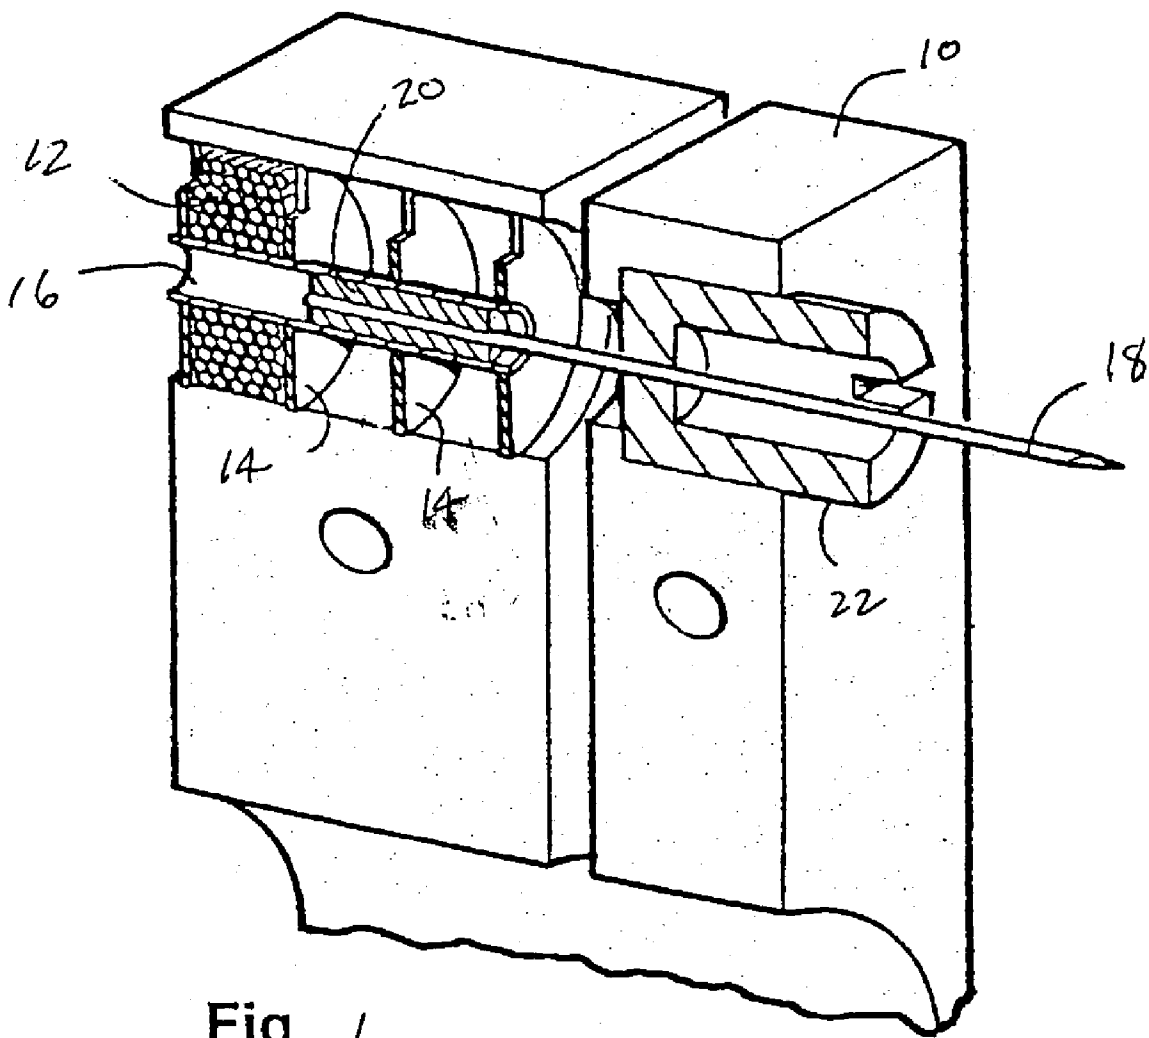


Fig 1

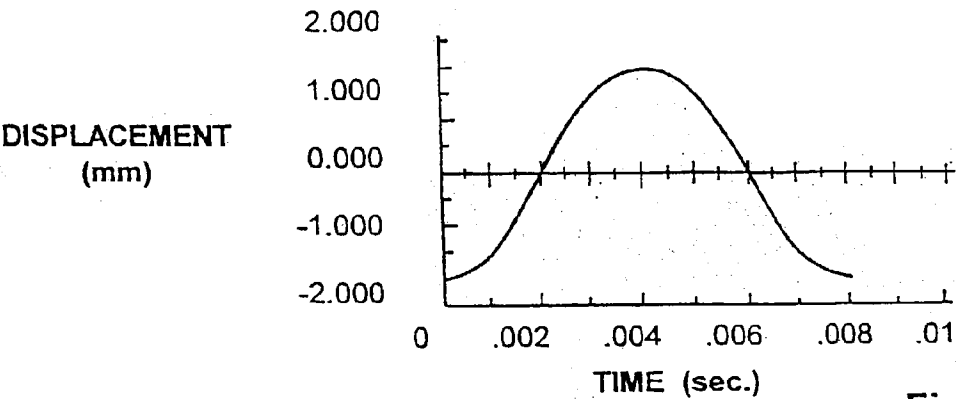


Fig. 2a

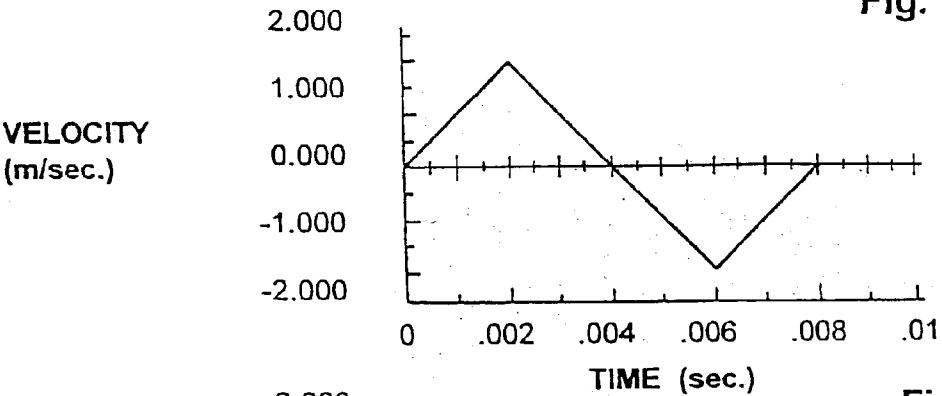


Fig. 2b

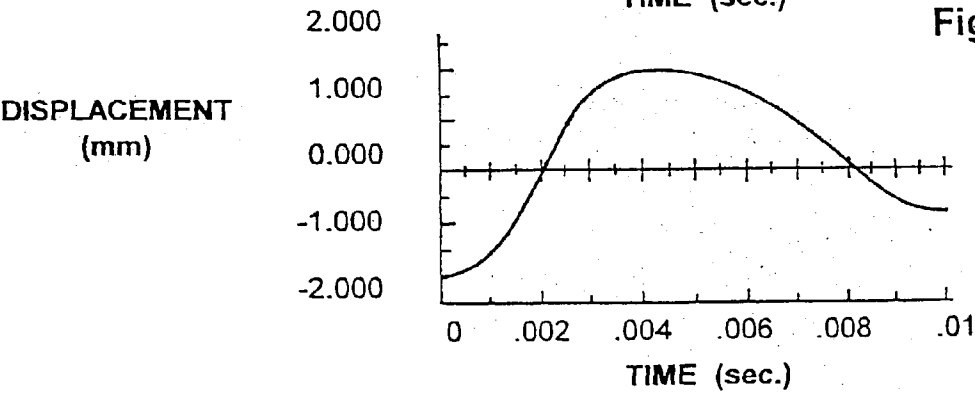


Fig. 2c

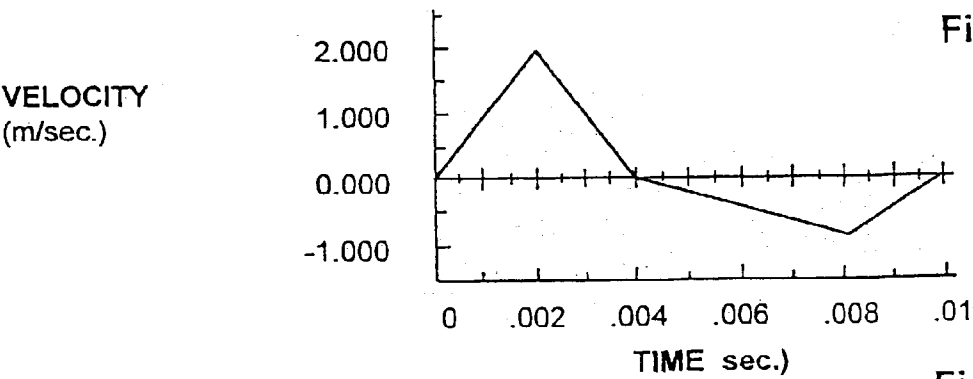


Fig. 2d

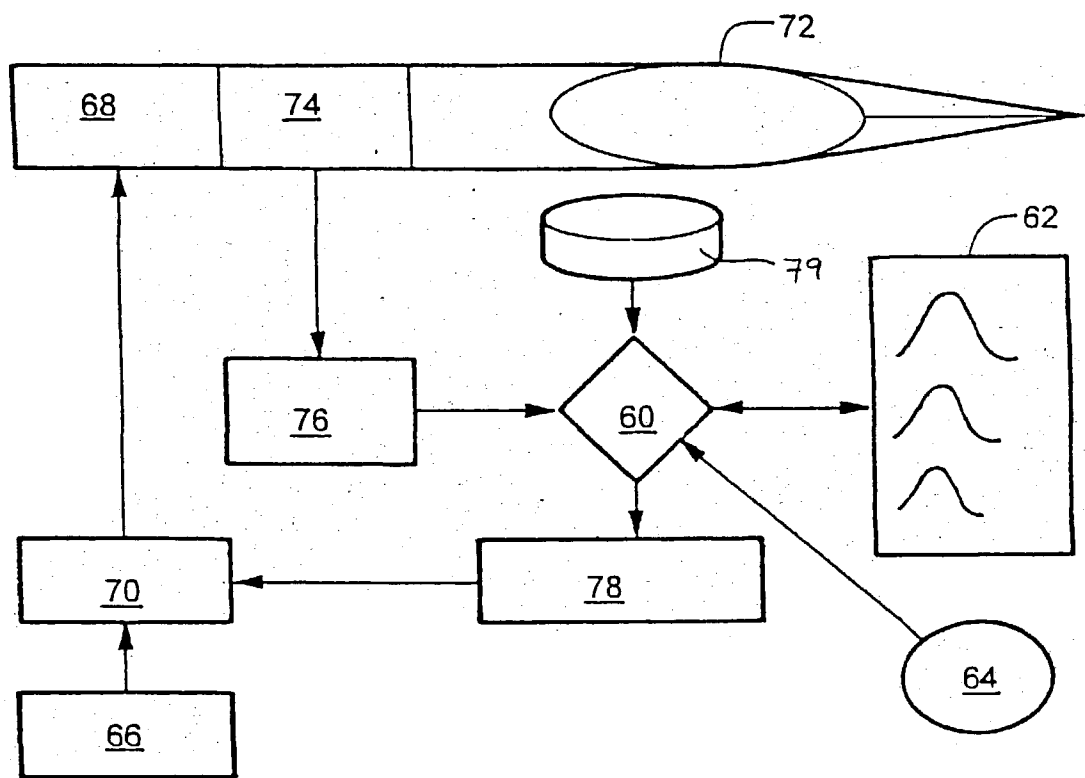


Fig. 3

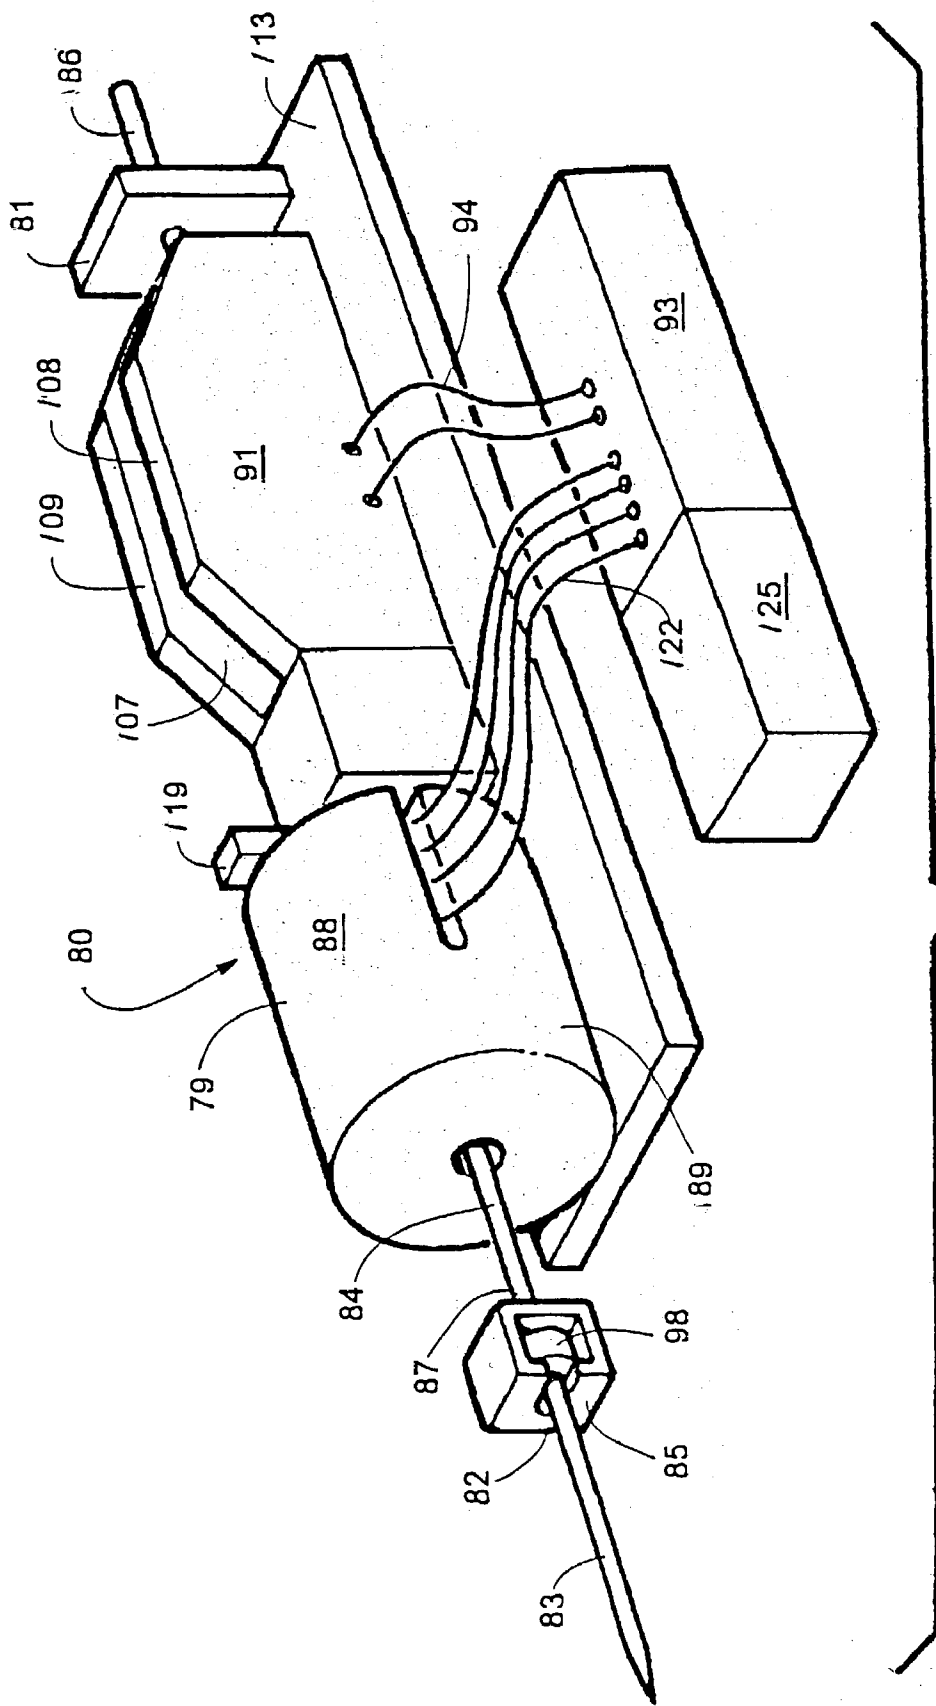


Fig. 4

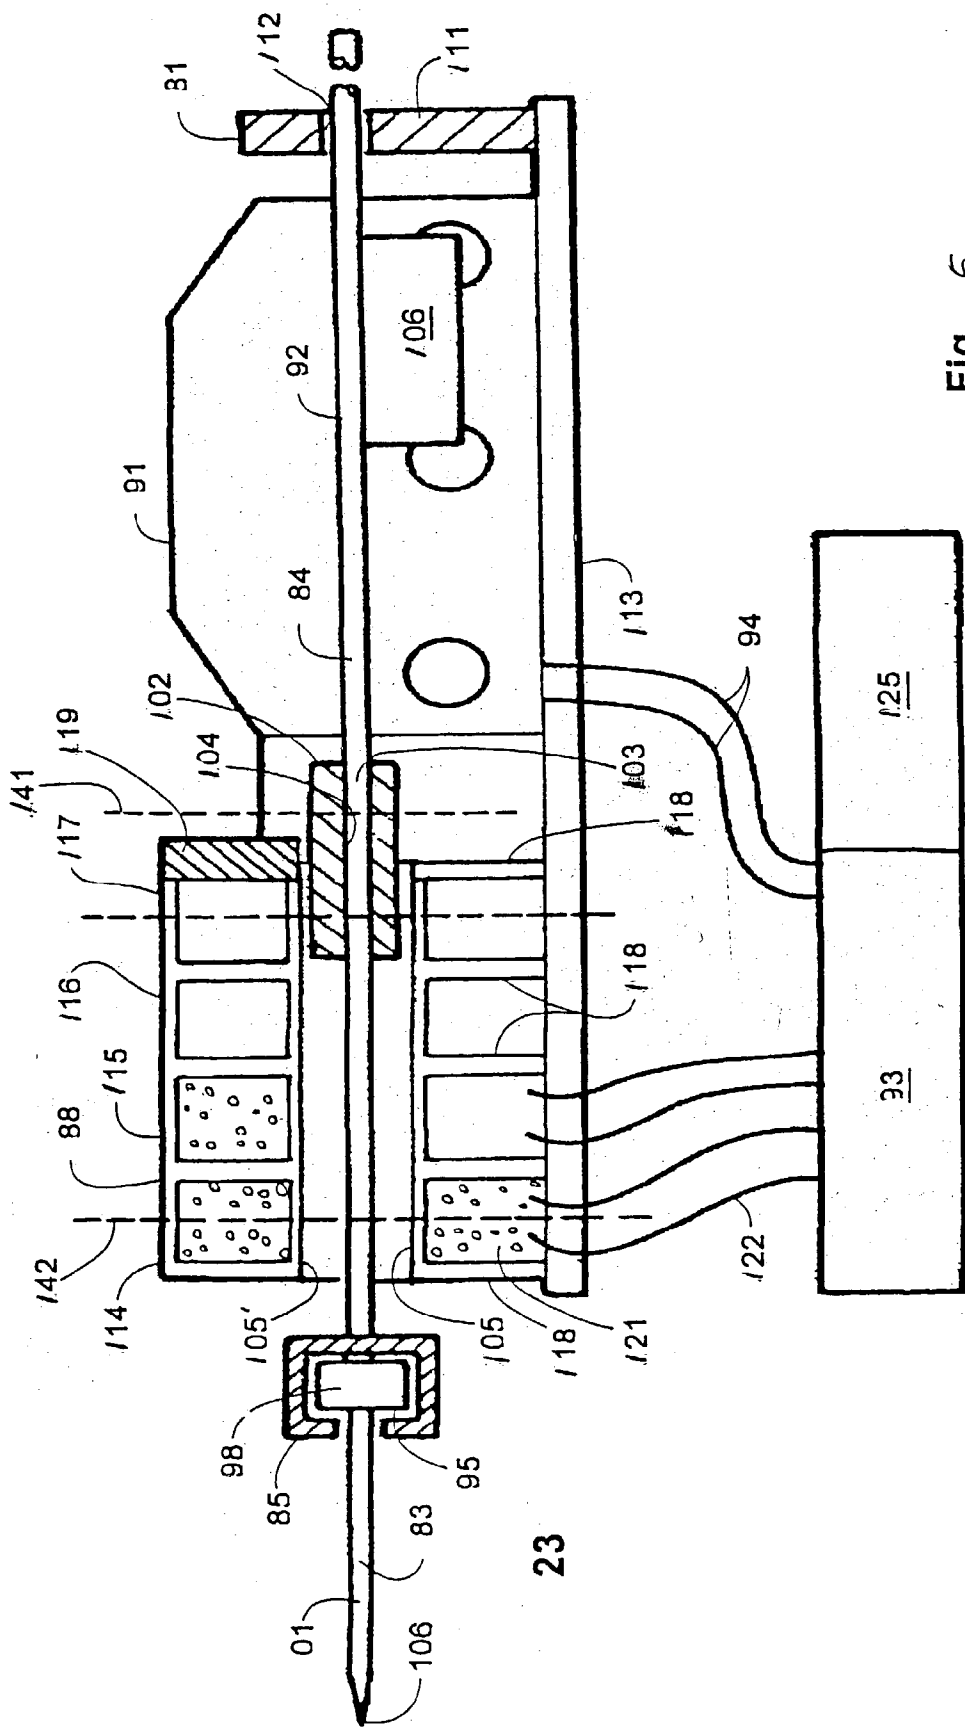


Fig. 5

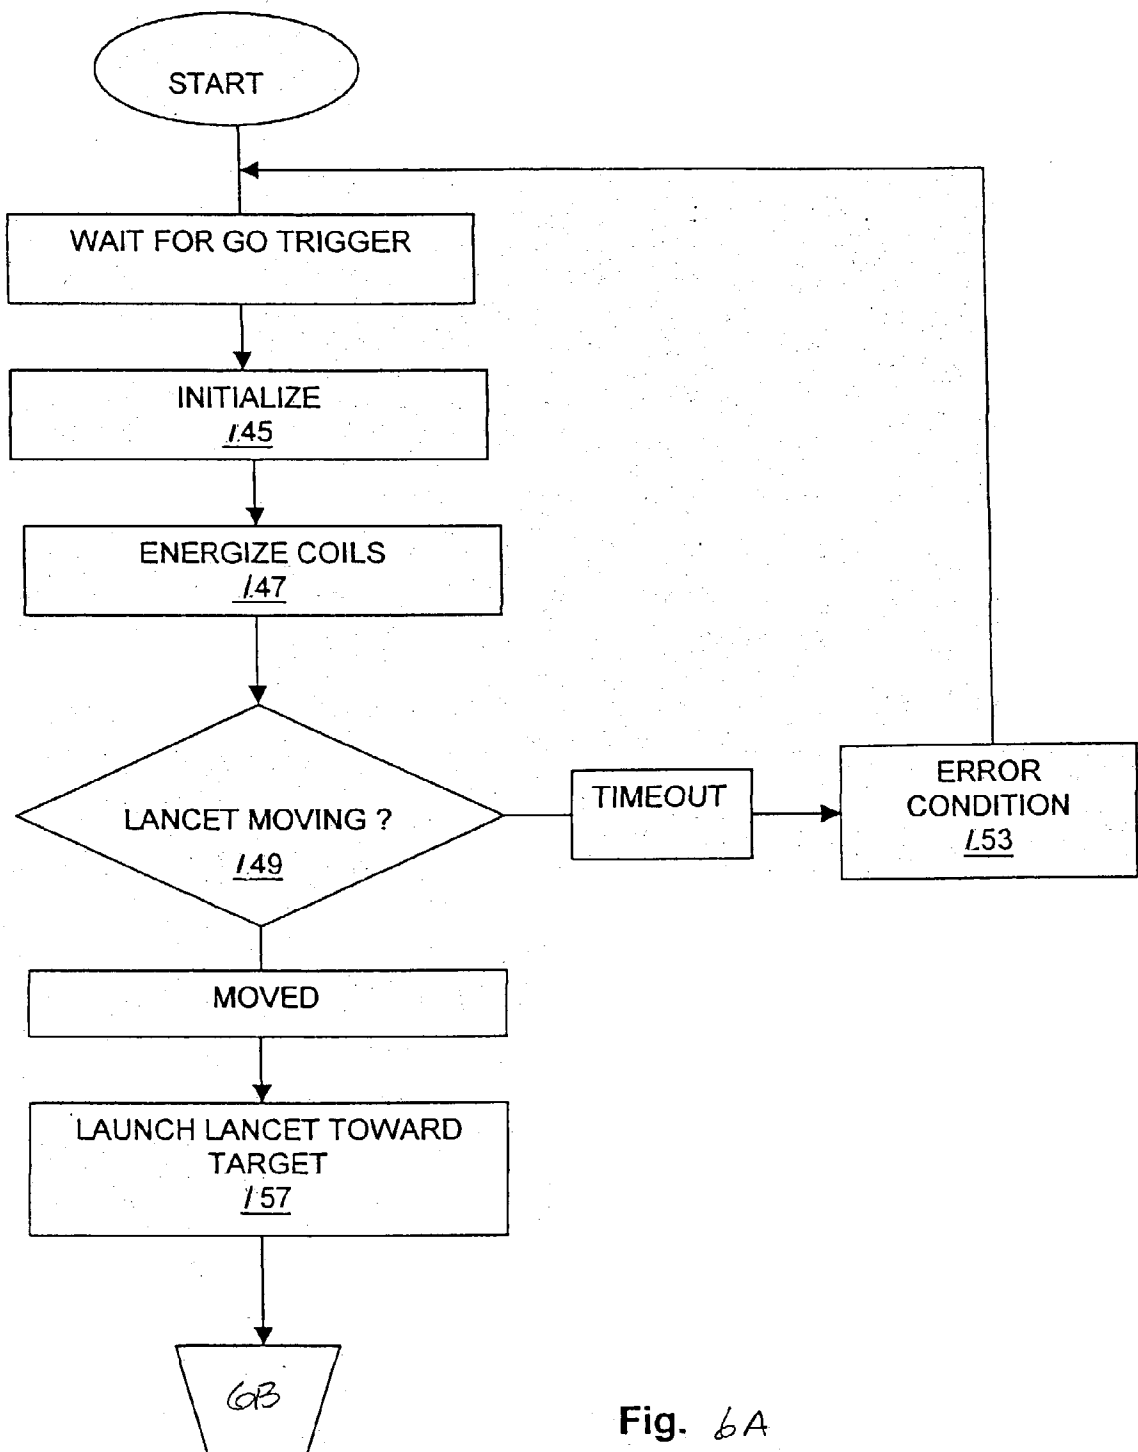


Fig. 6A

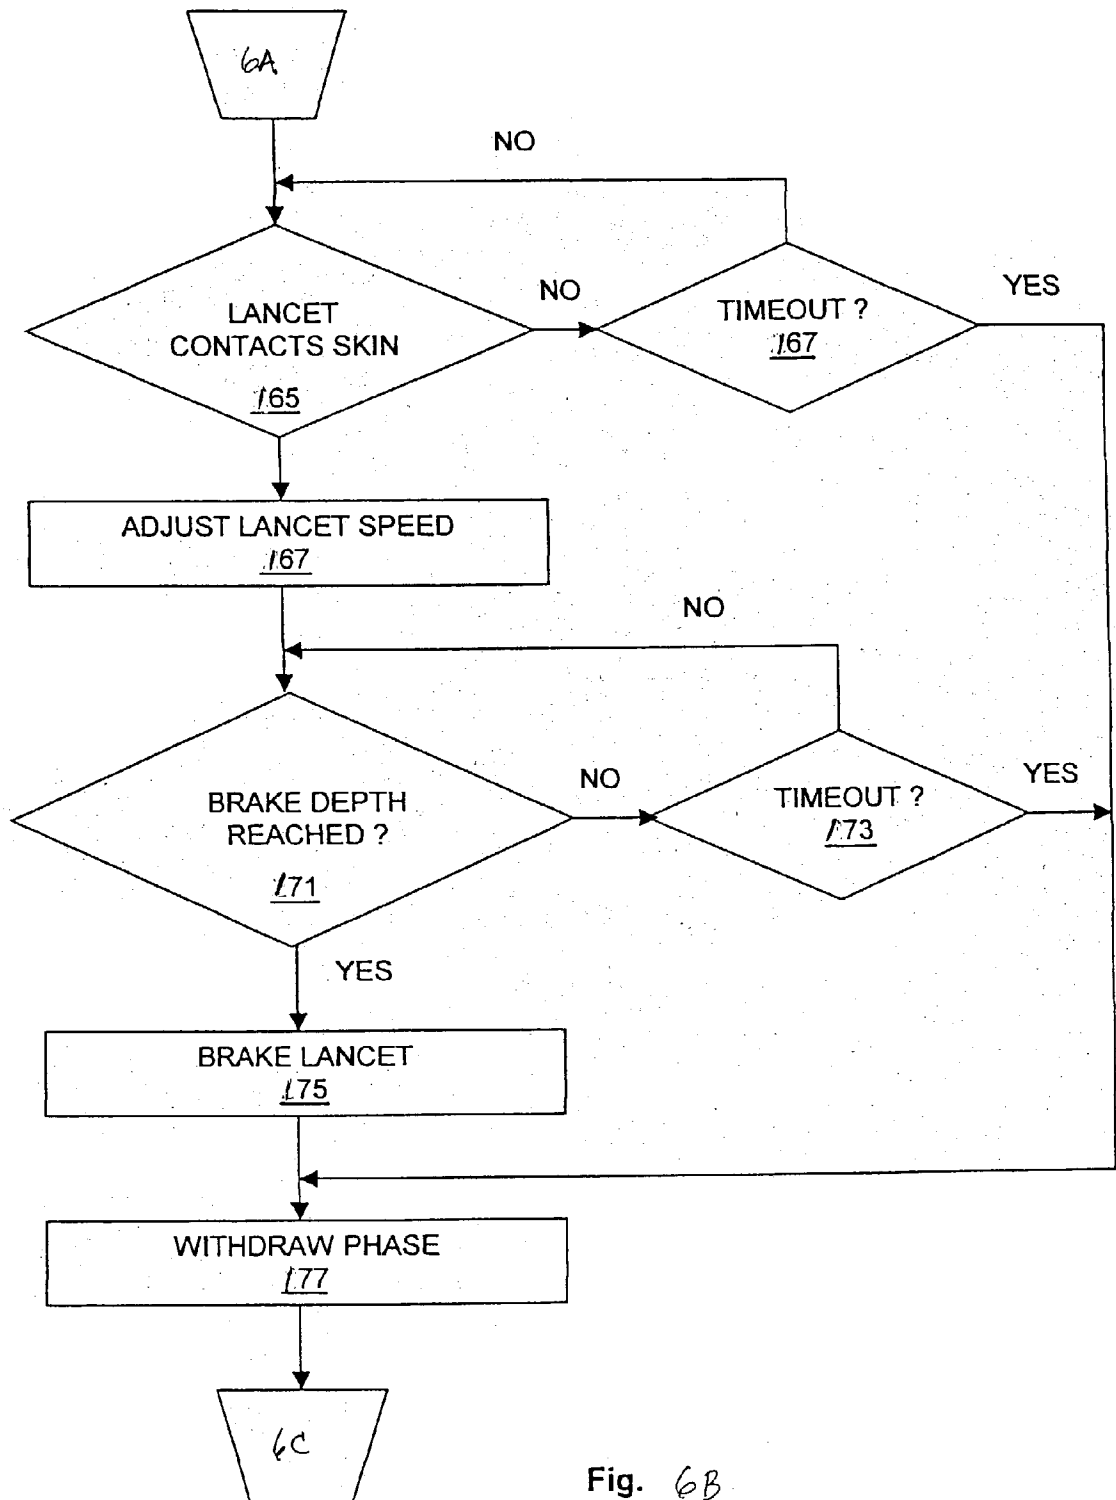


Fig. 6B

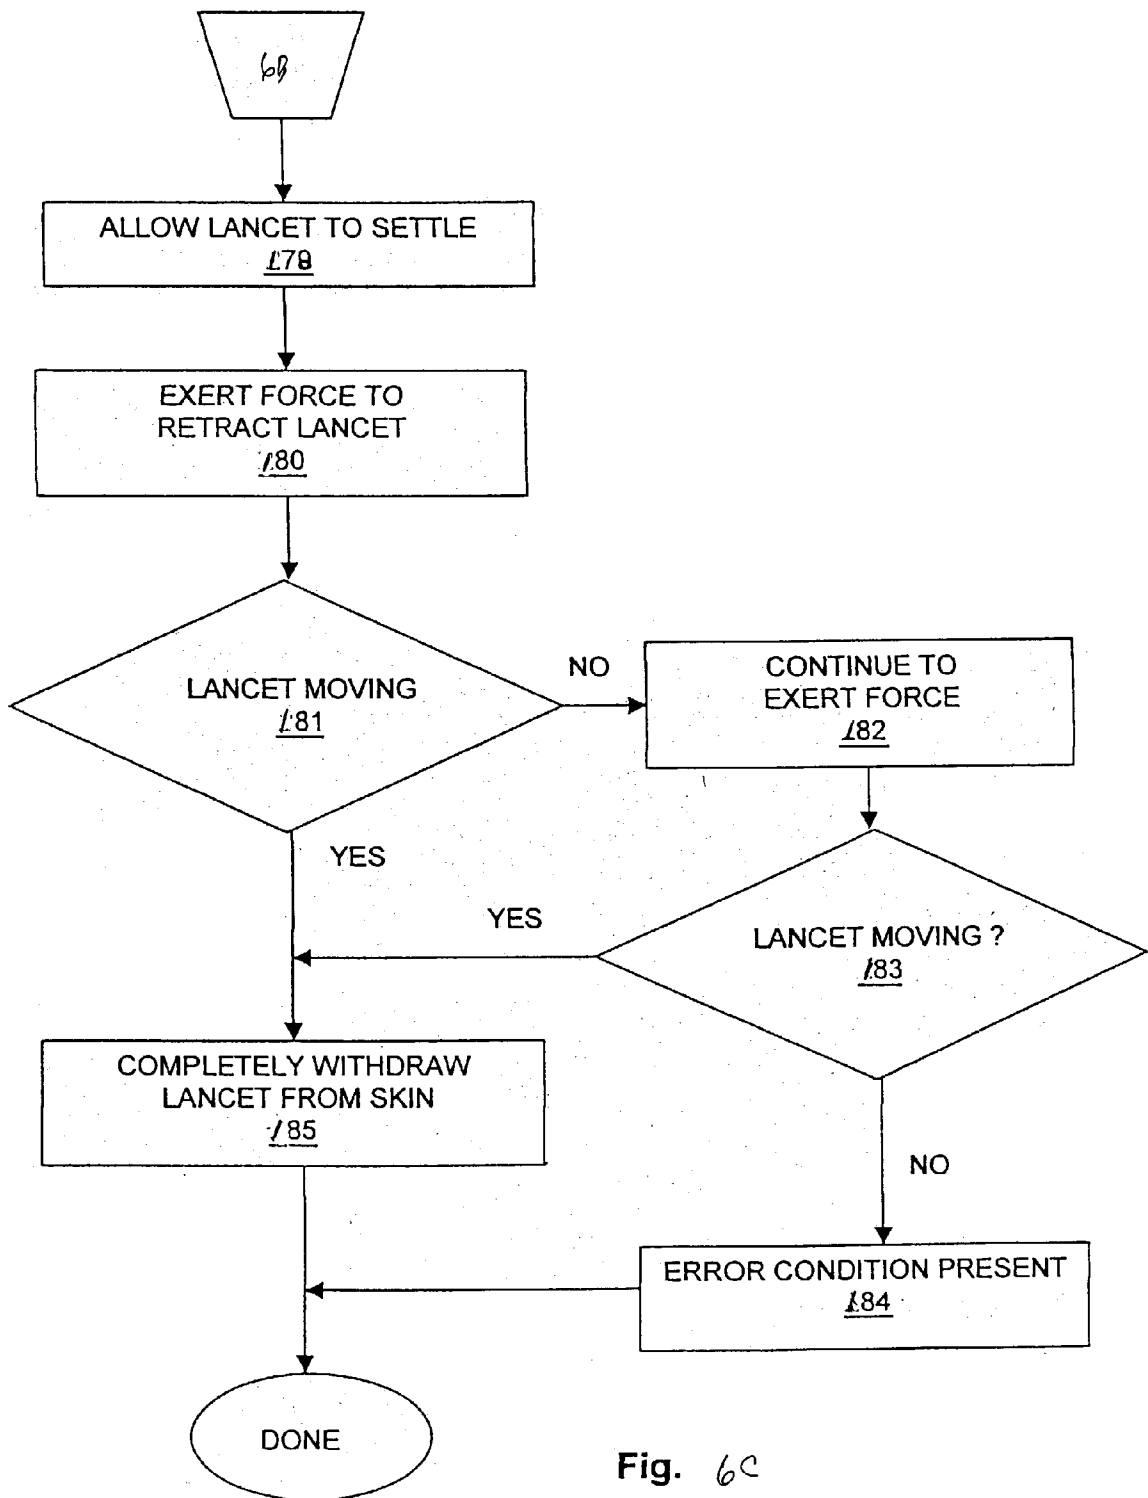


Fig. 6c

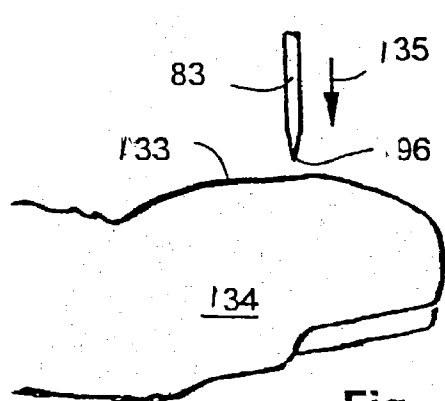


Fig. 7

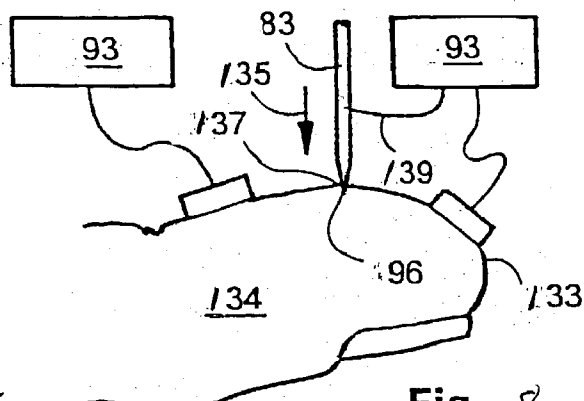


Fig. 8

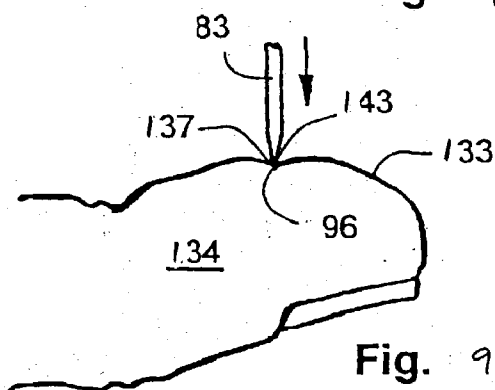


Fig. 9

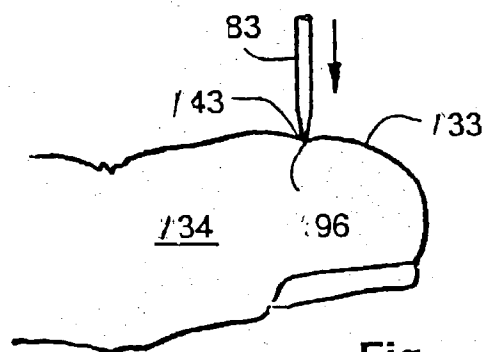


Fig. 10

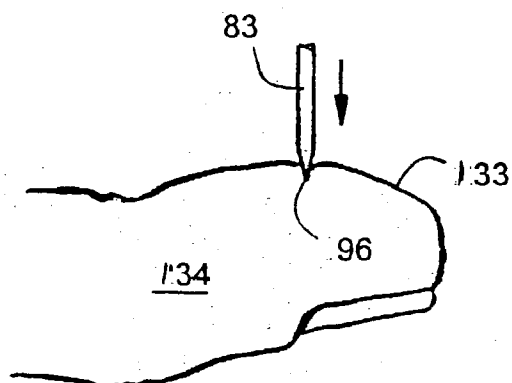


Fig. 11

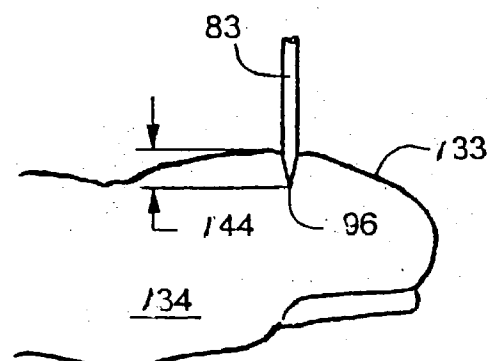


Fig. 12

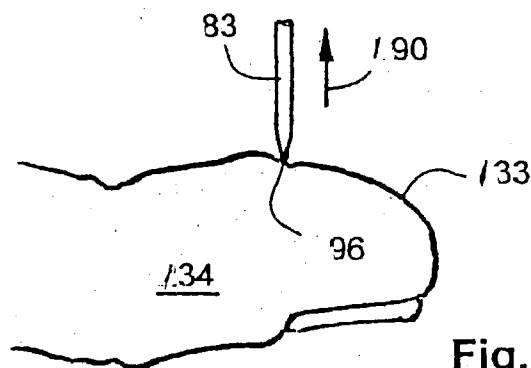


Fig. 13

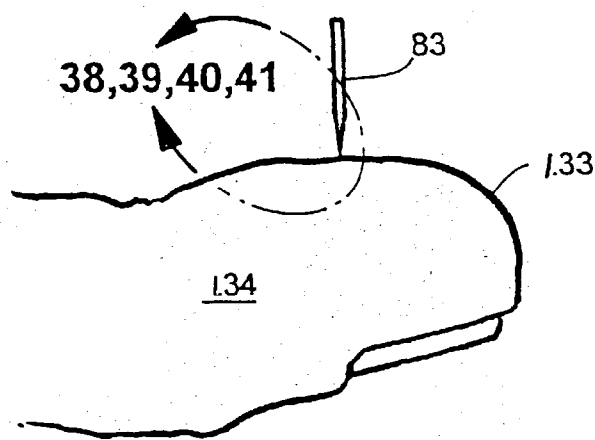


Fig. 14

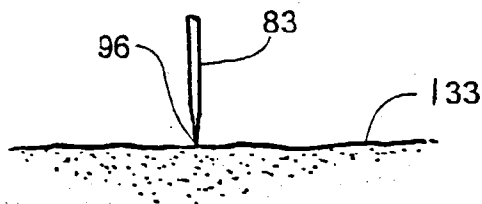


Fig. 15

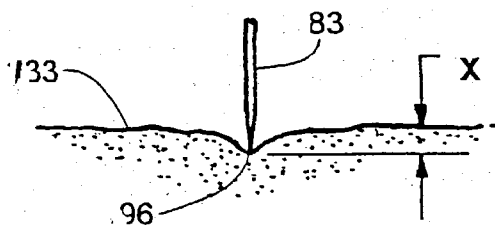


Fig. 16

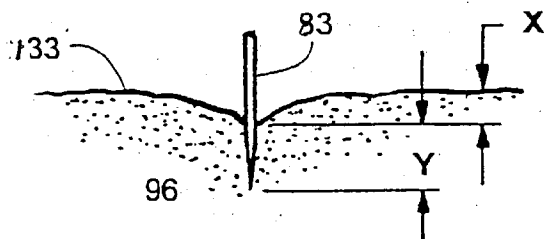


Fig. 17

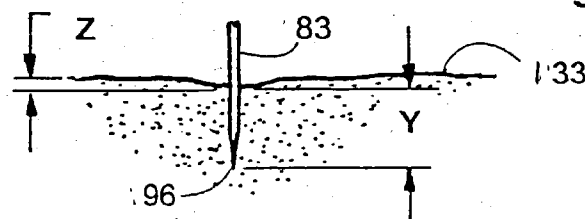


Fig. 18

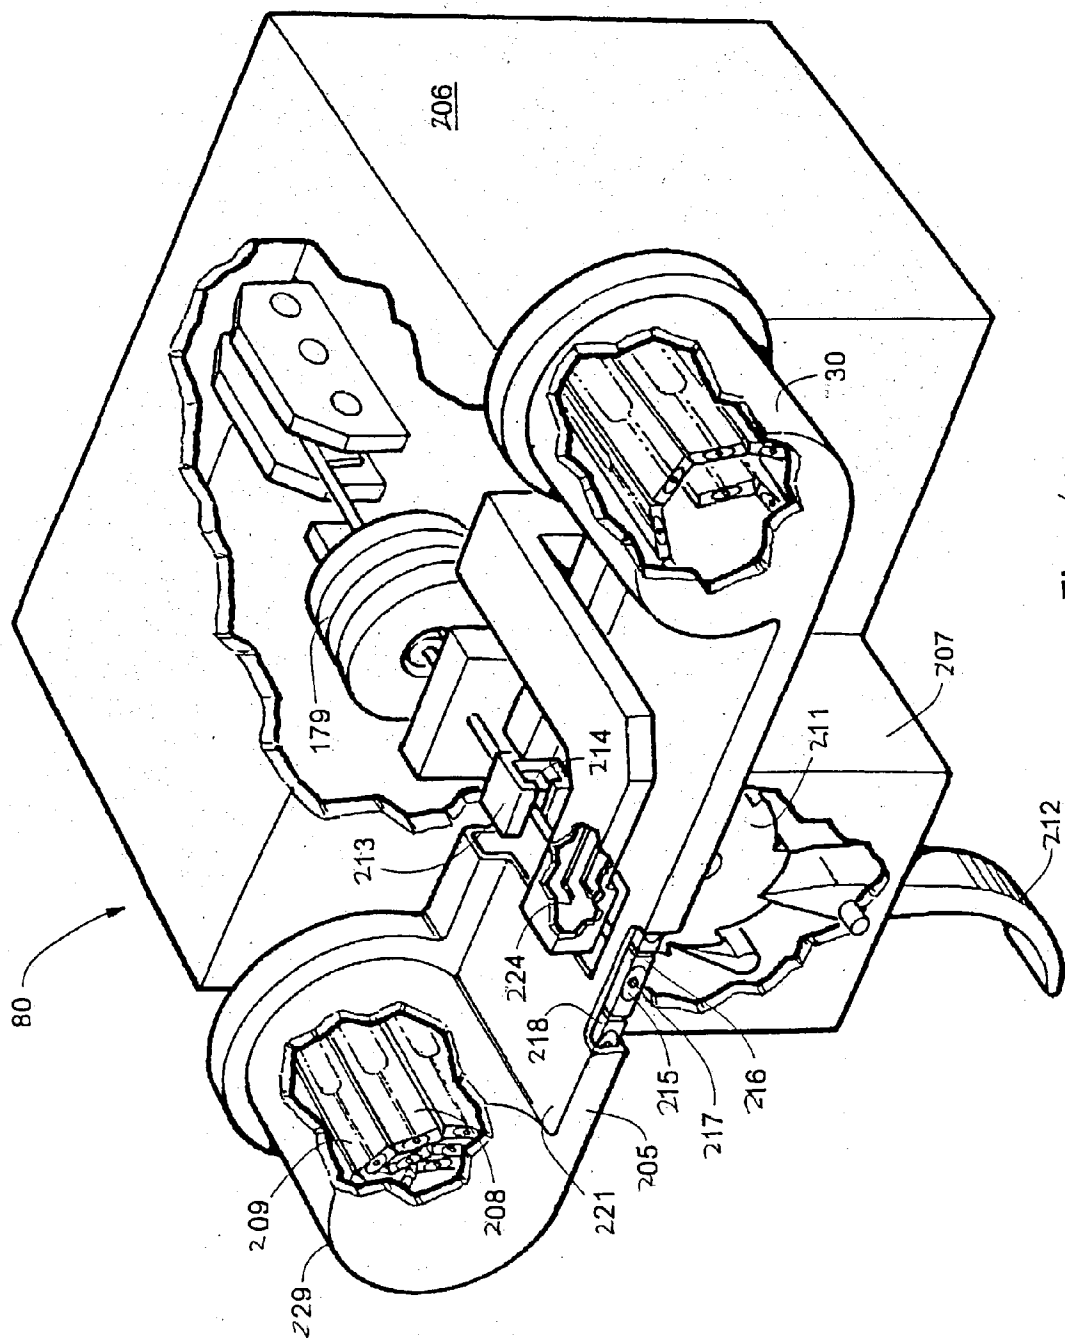


Fig. 19

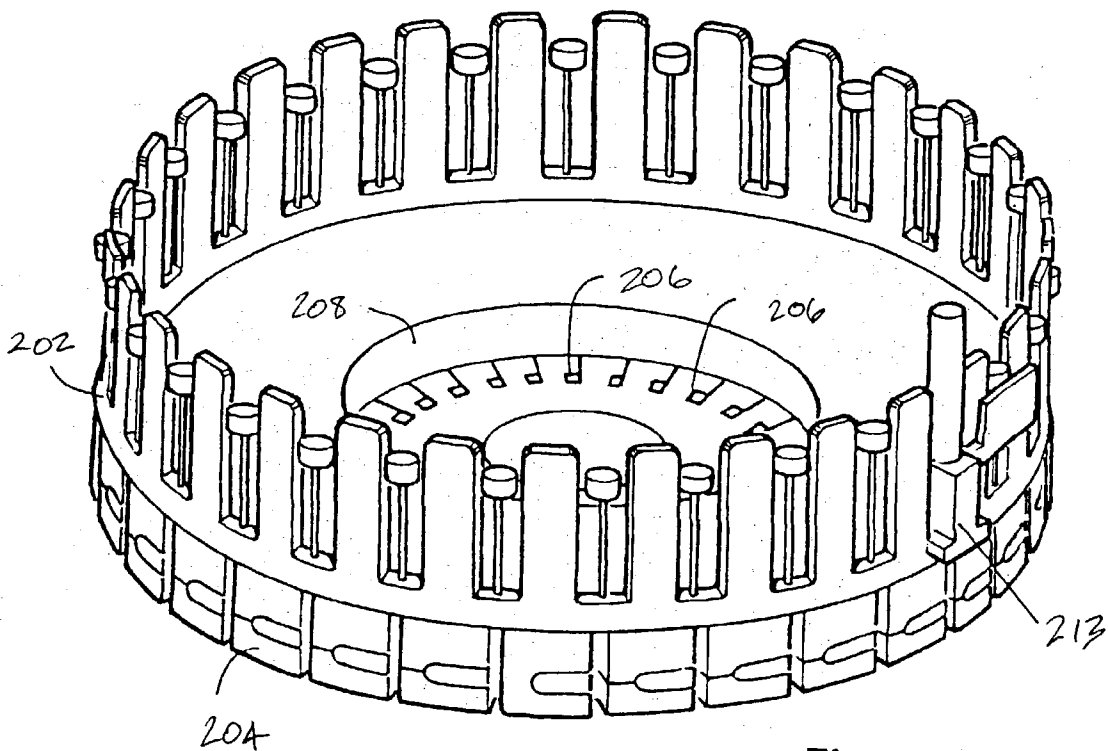


Fig. 20

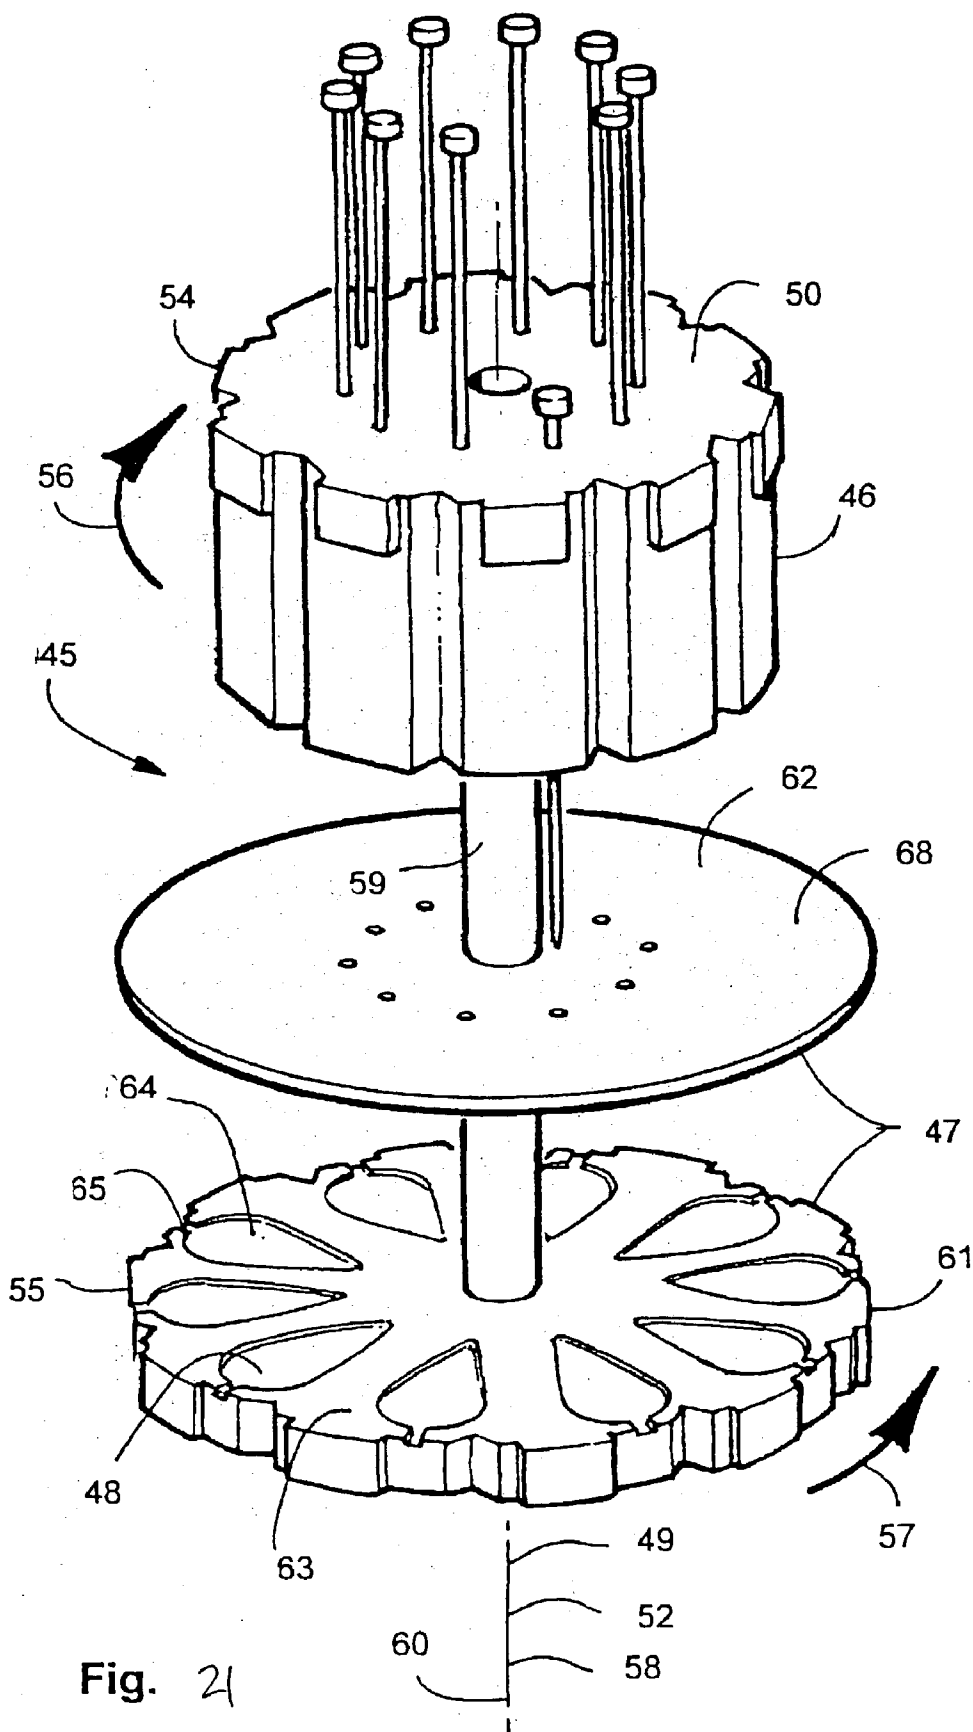
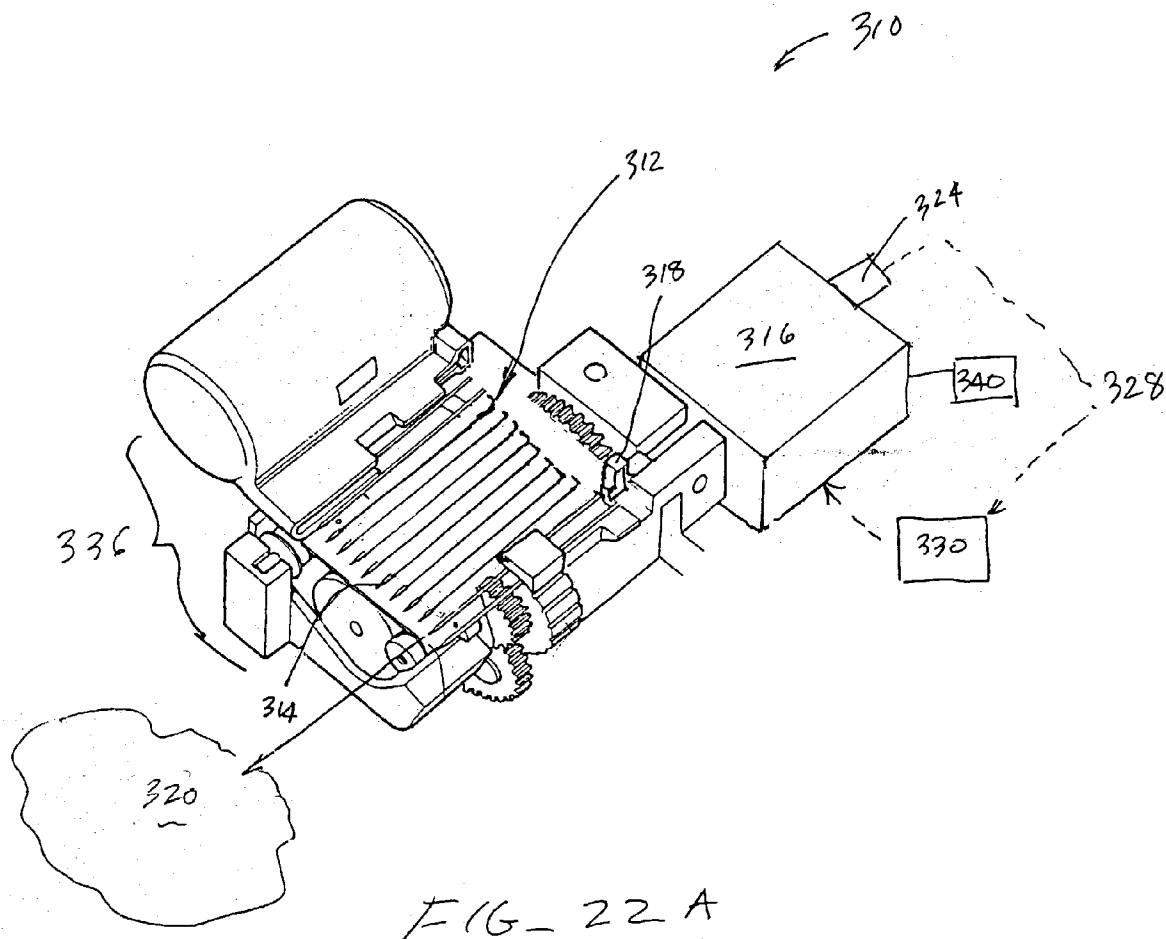


Fig. 21






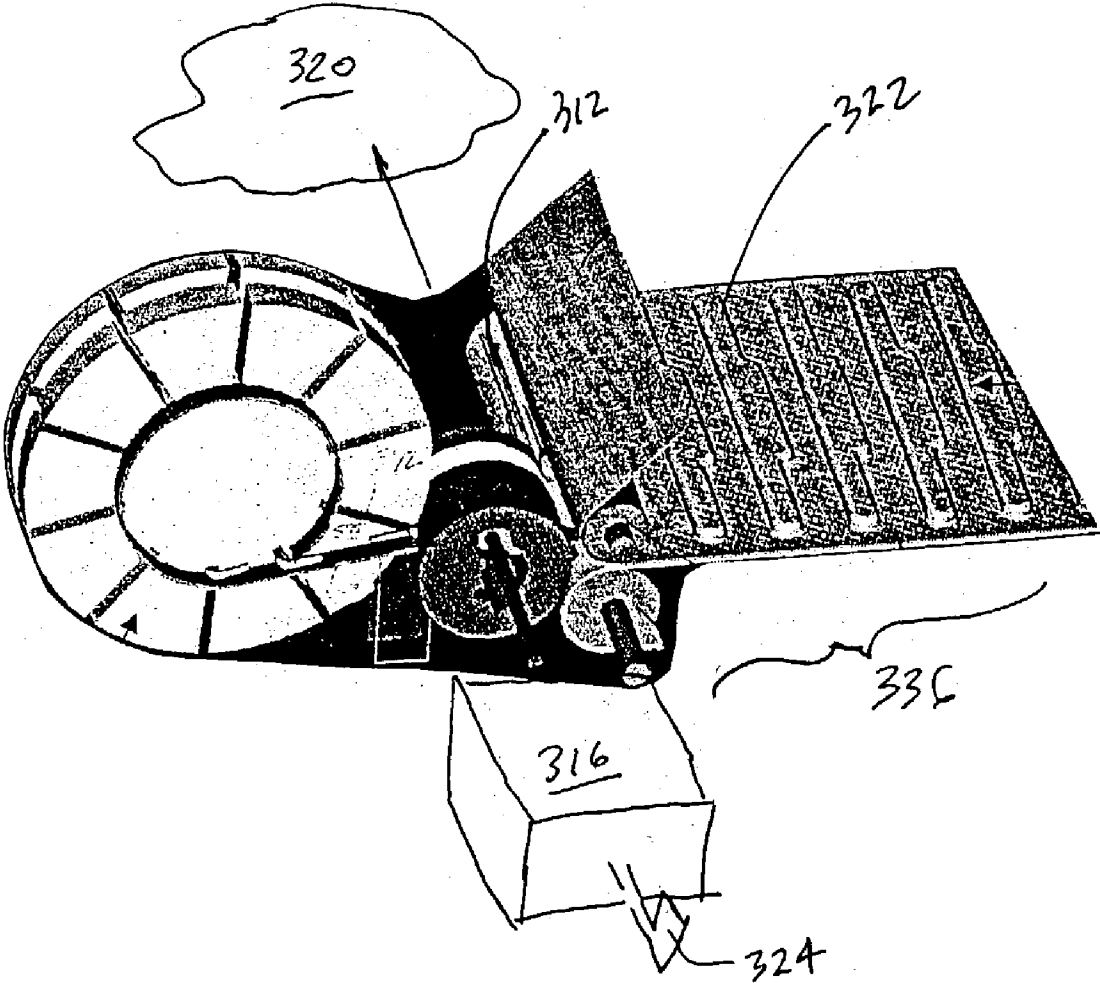


FIG-22B

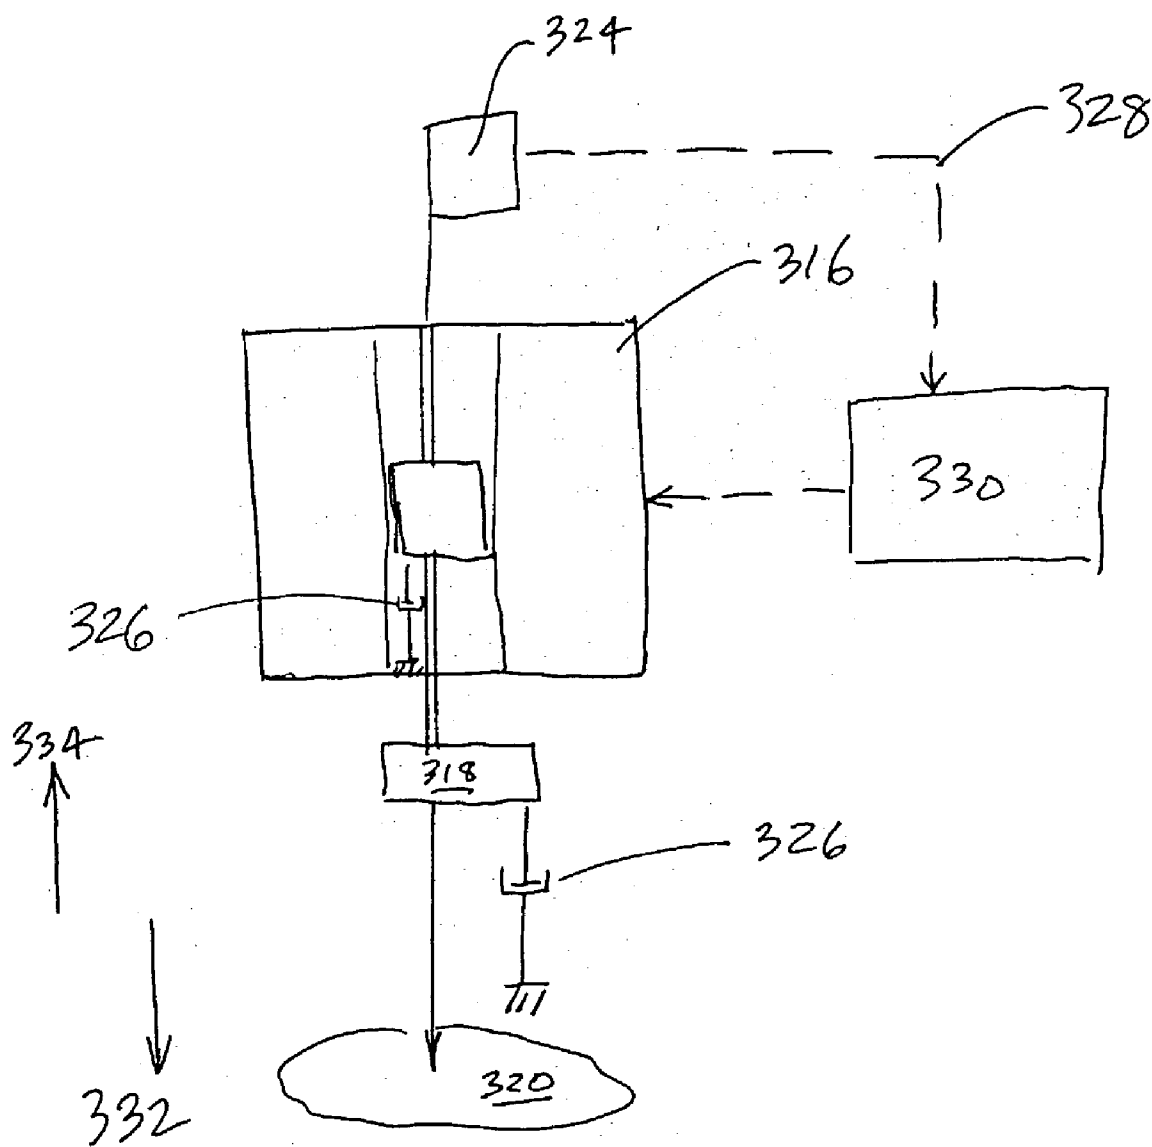

FIG\_22C

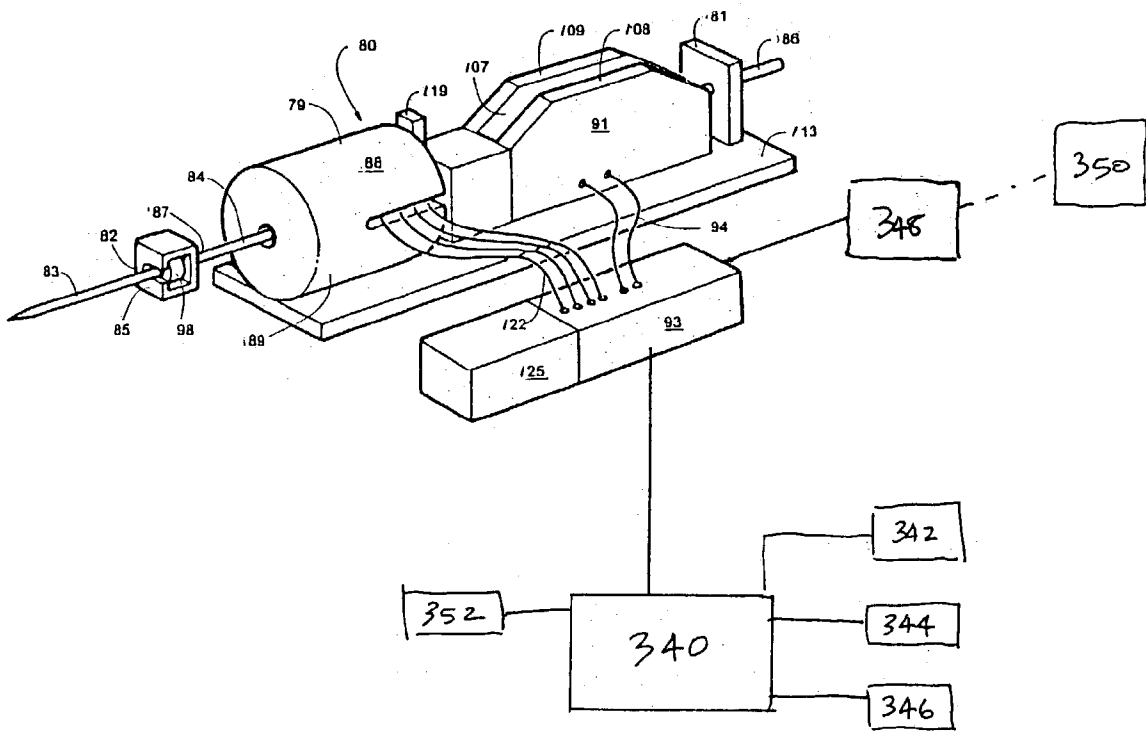

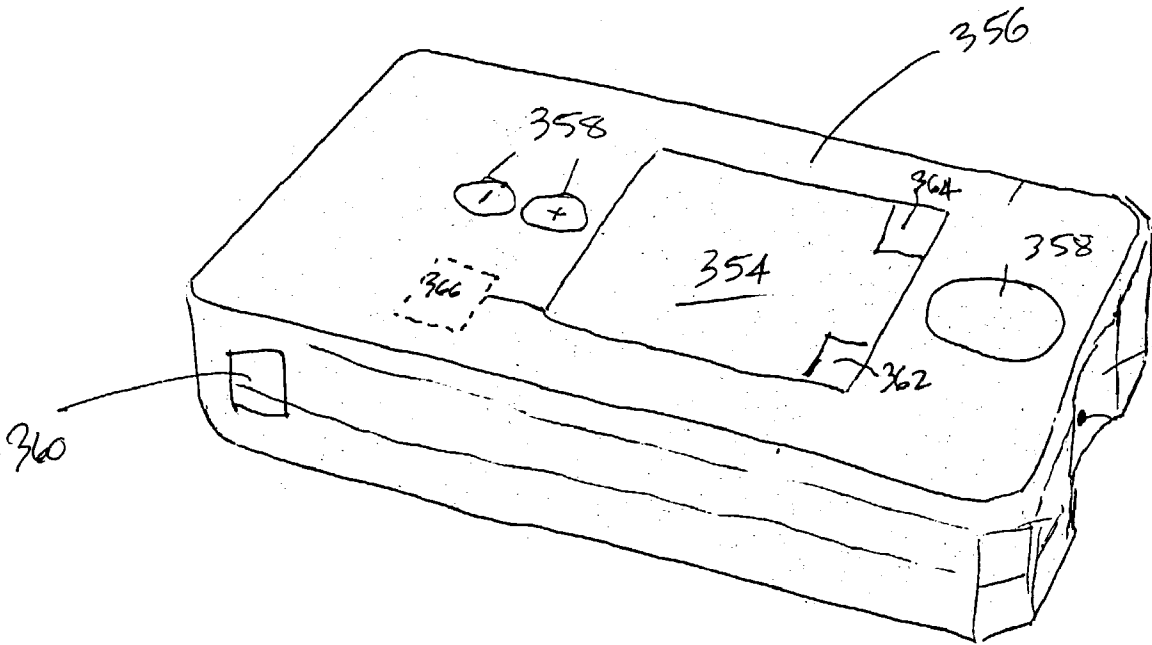

FIG\_23B

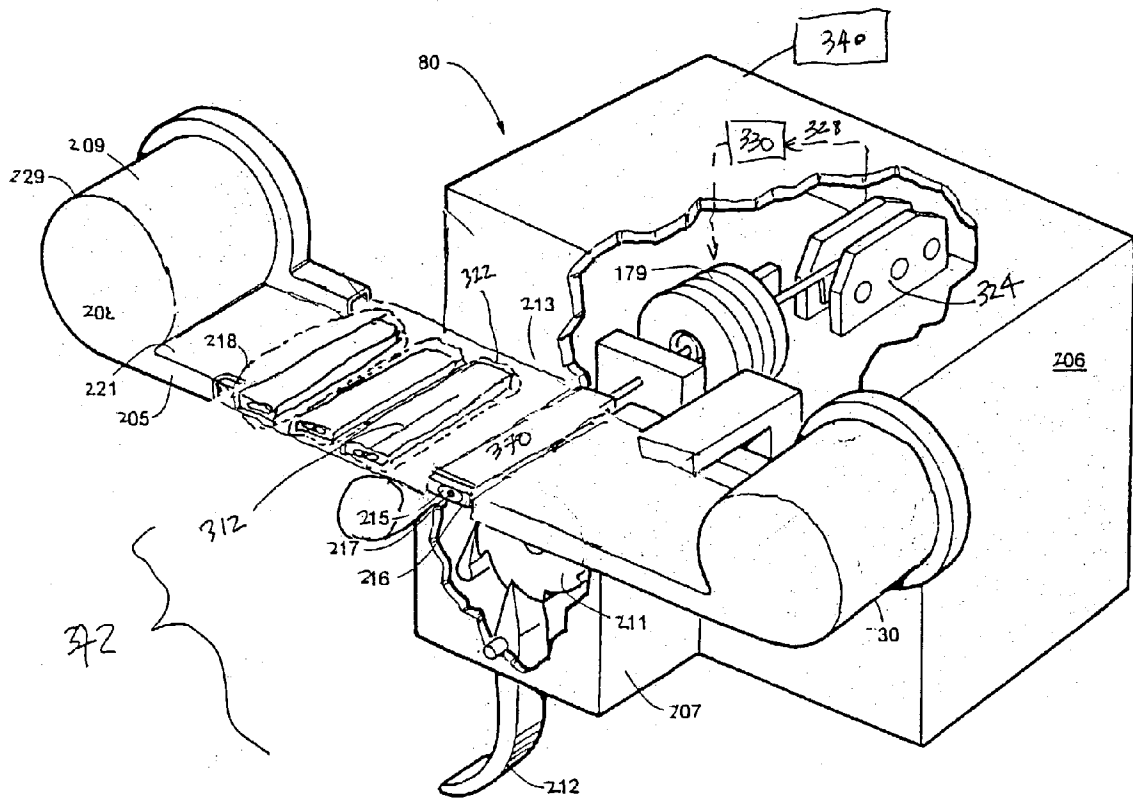


FIG-24


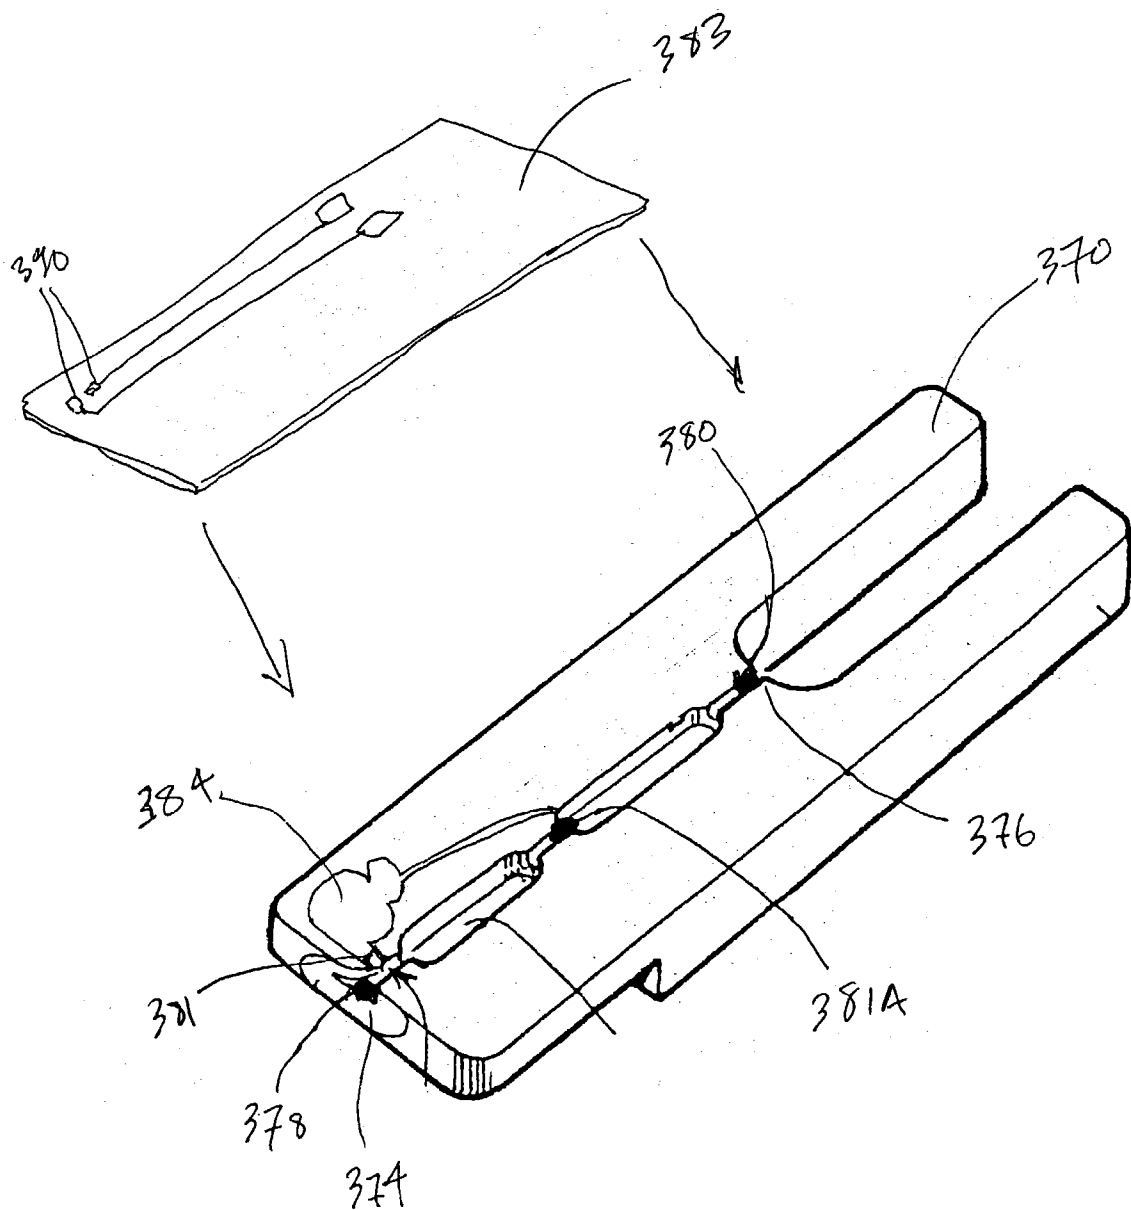


FIG 25

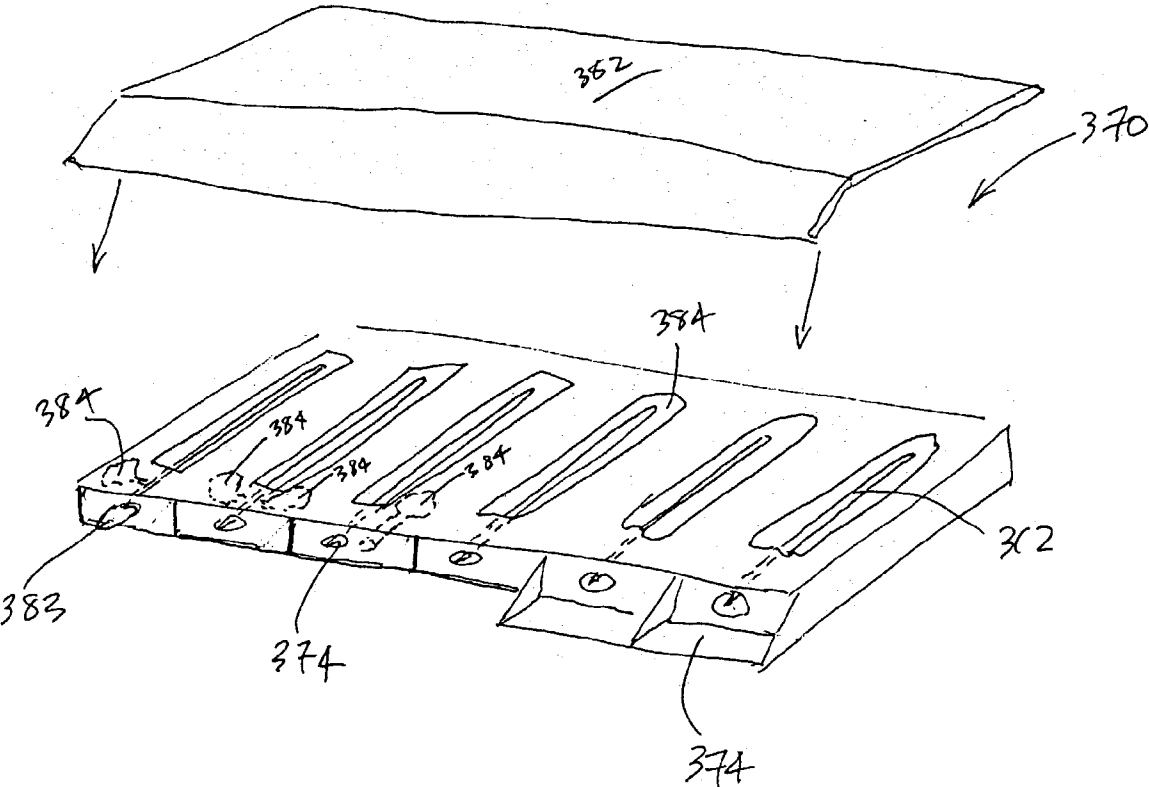

FIG\_26


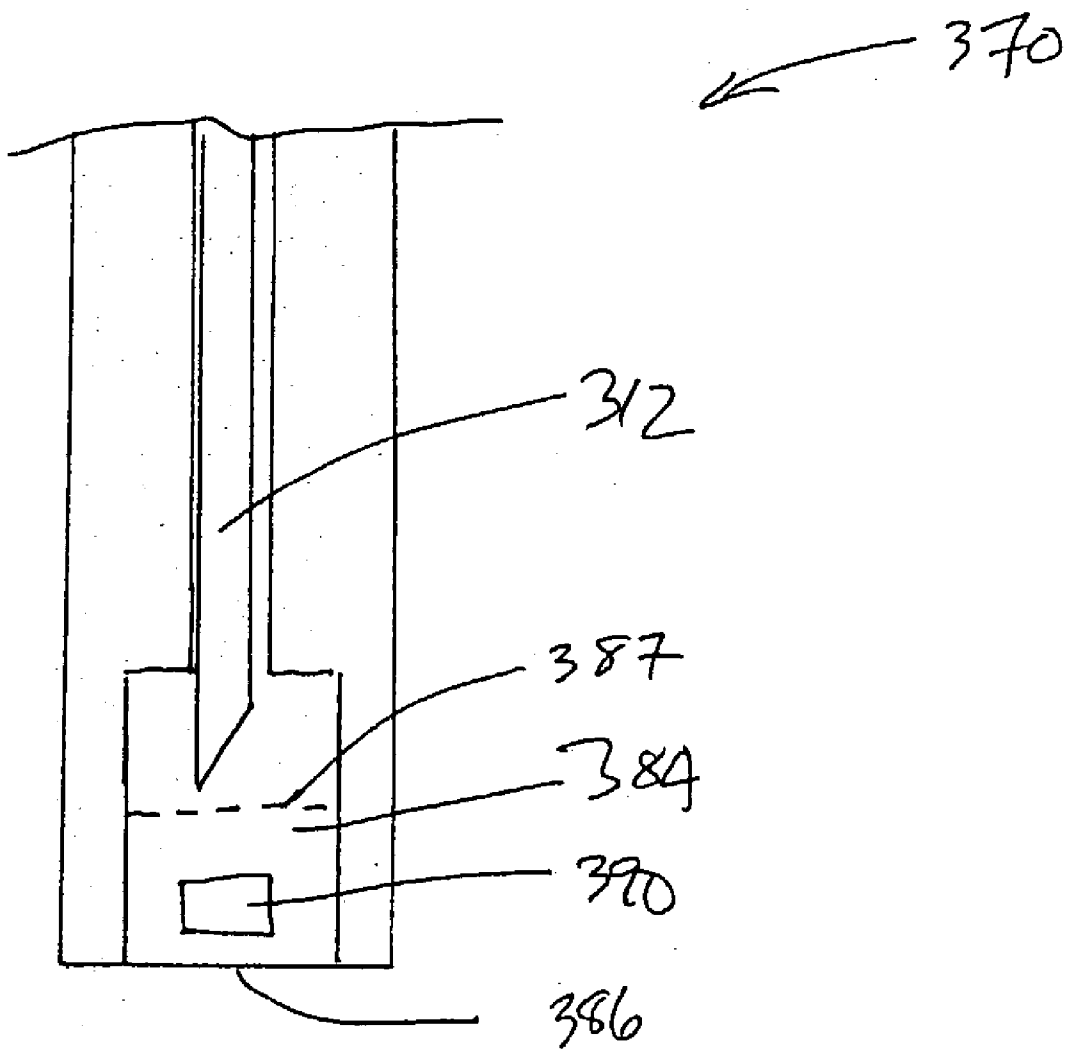


FIG-27

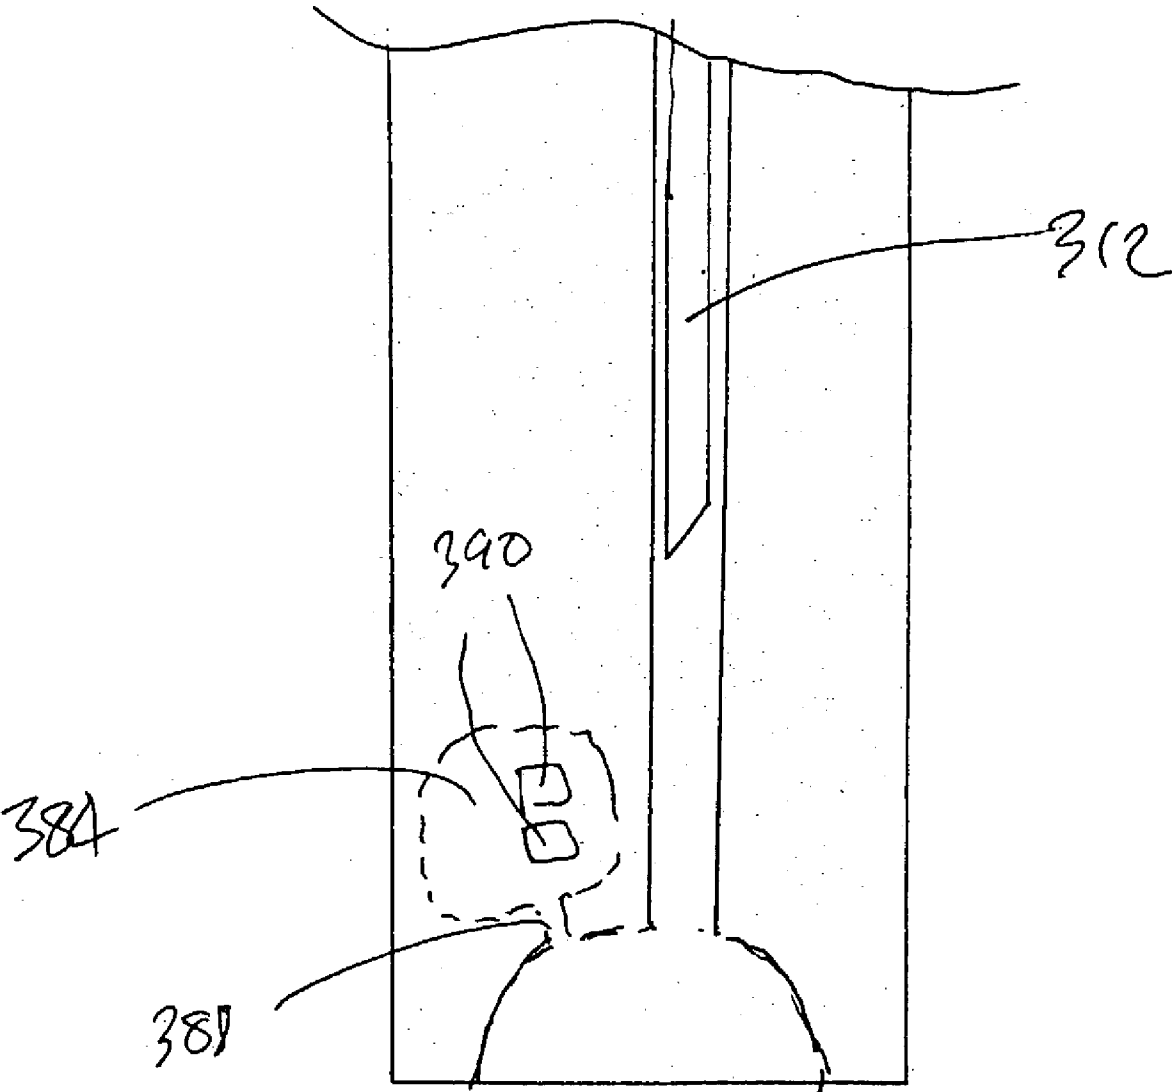

F 6 - 28

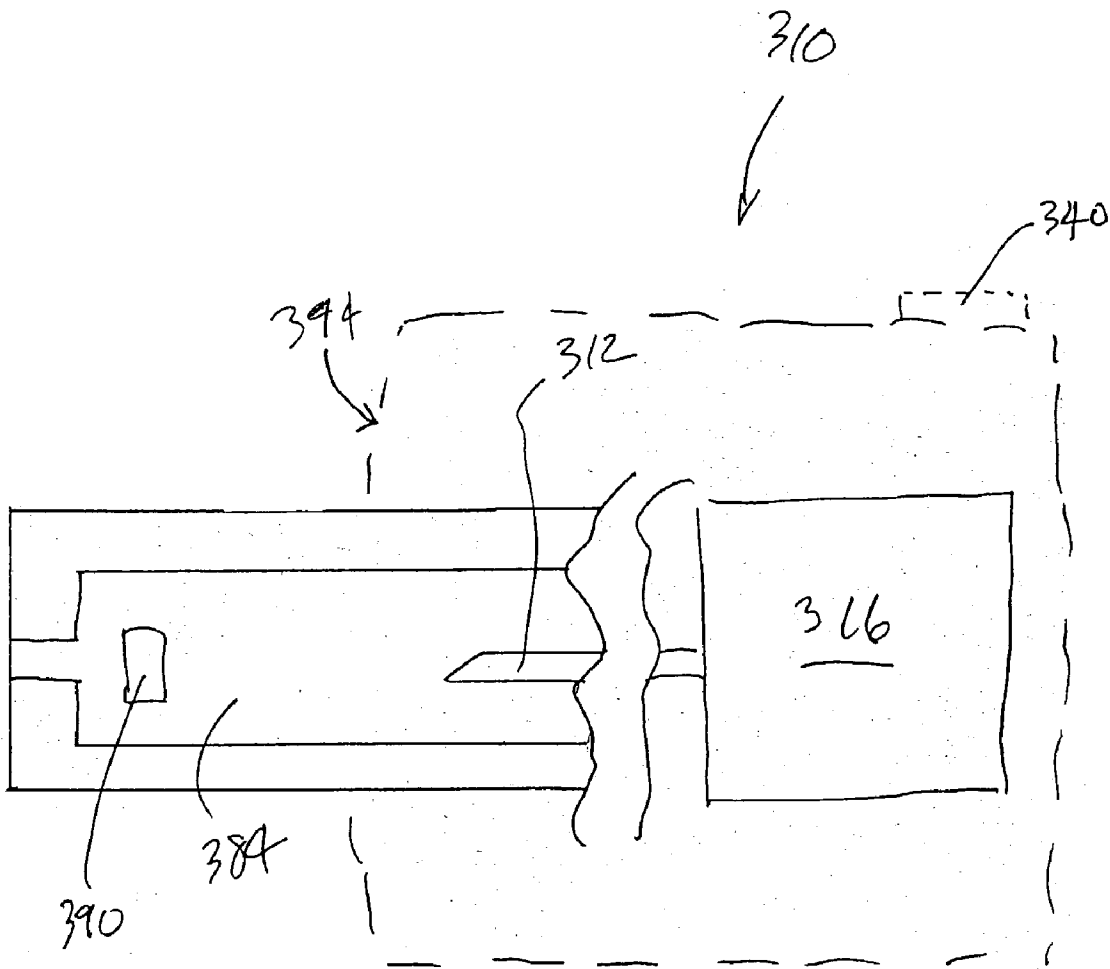


FIG. 29

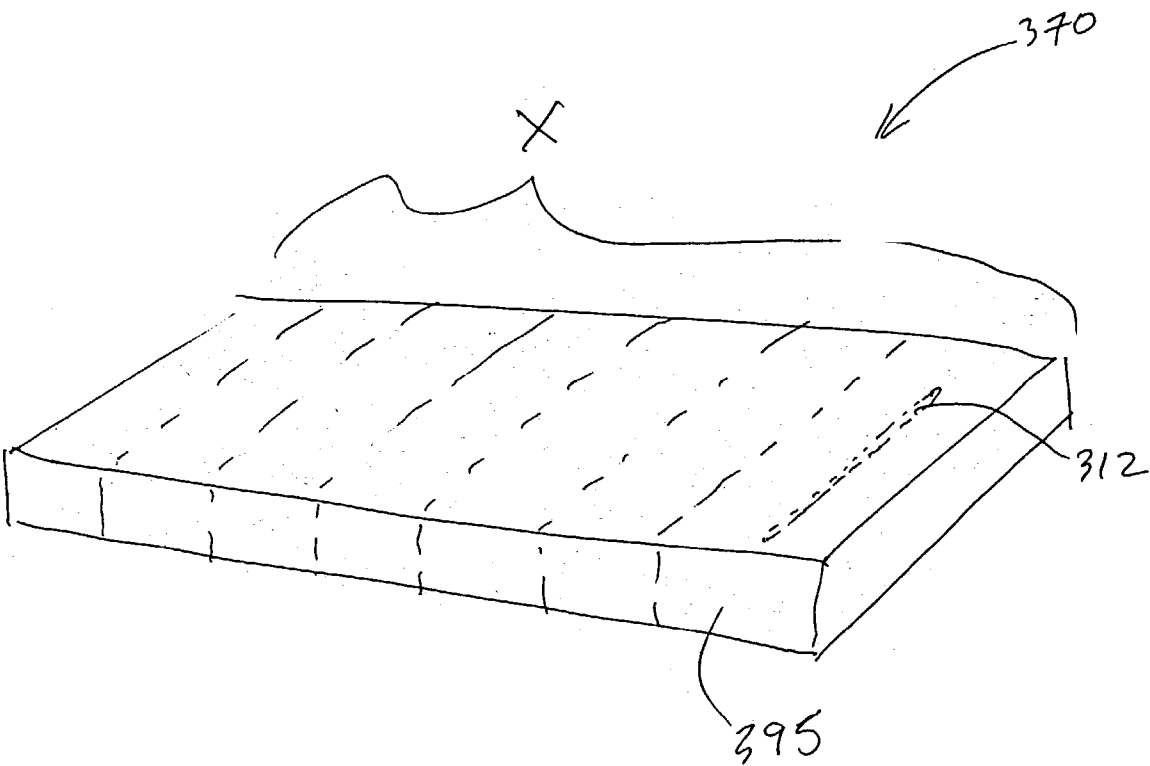


FIG. 30



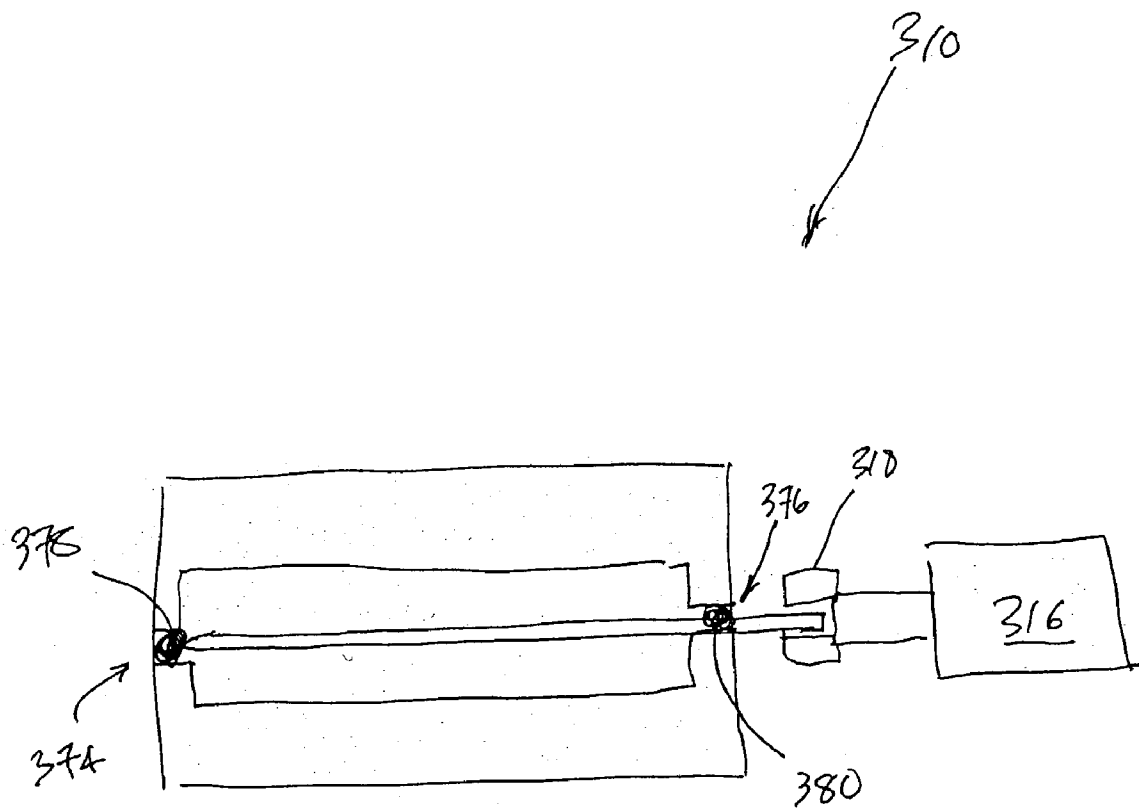



FIG-31

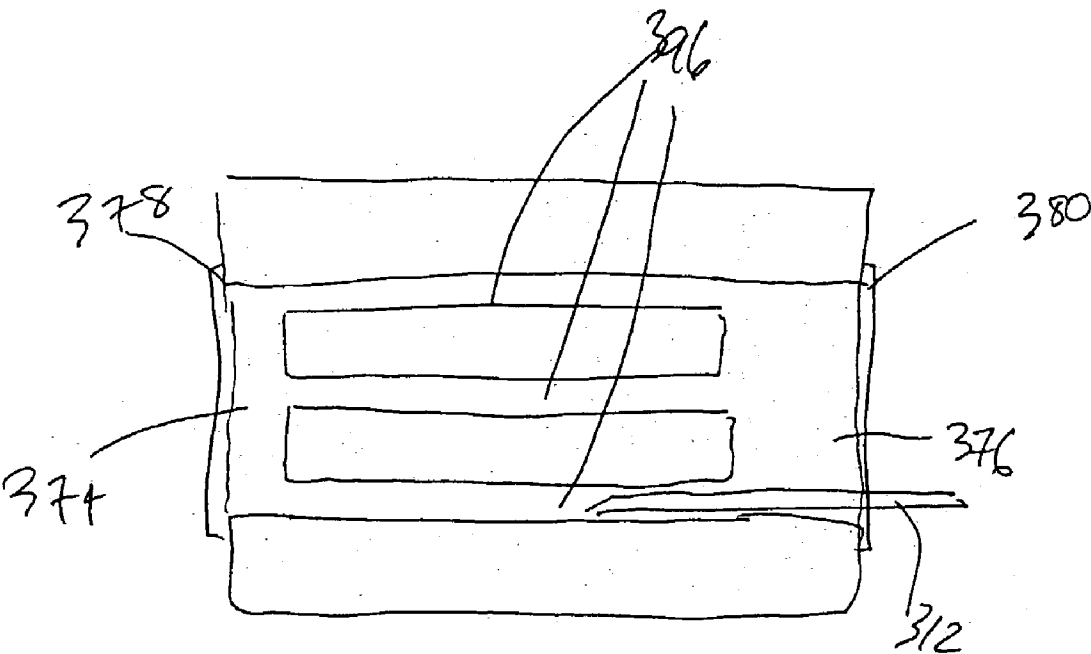

F 16-32

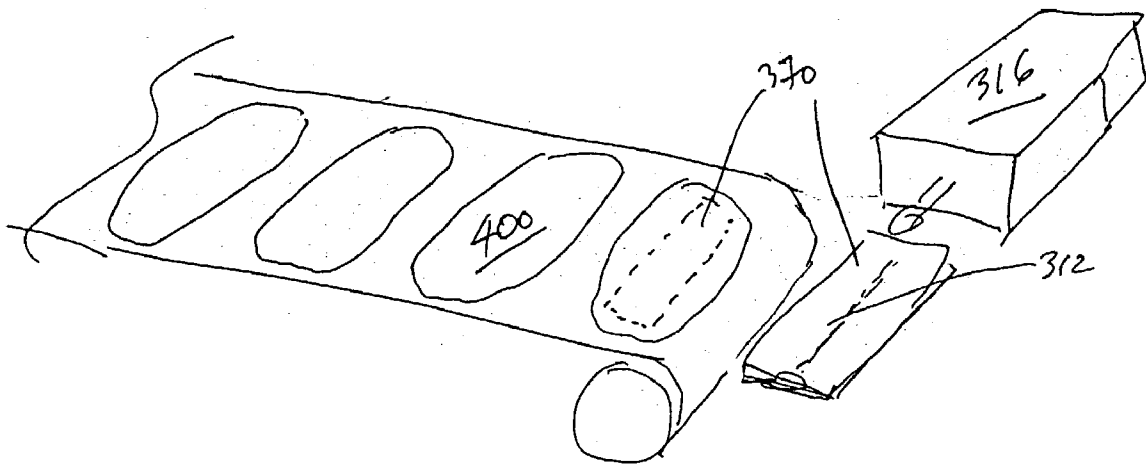

FIG\_33

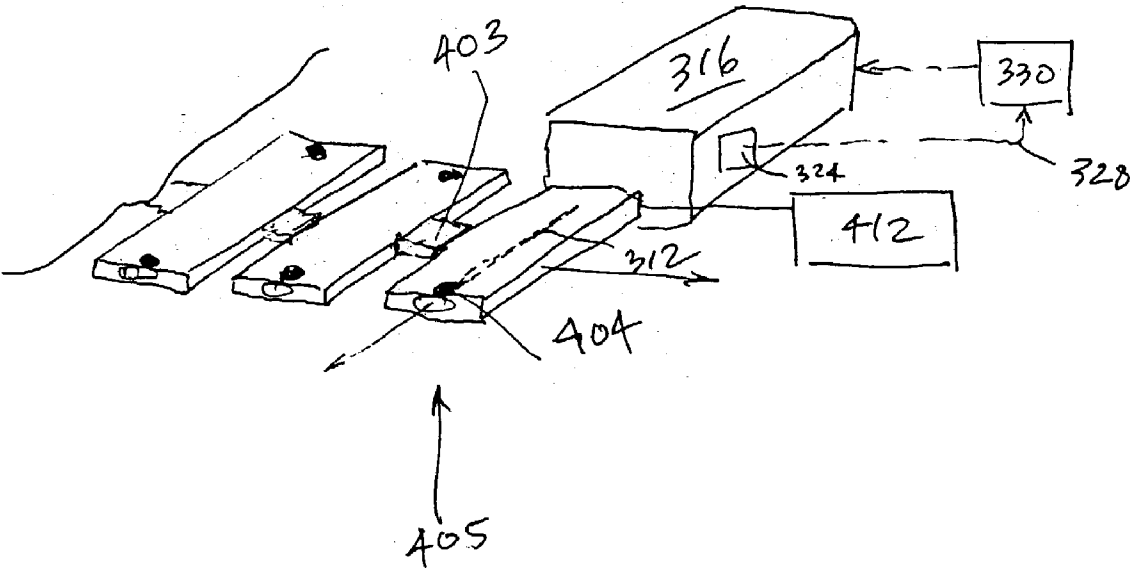

F16-34

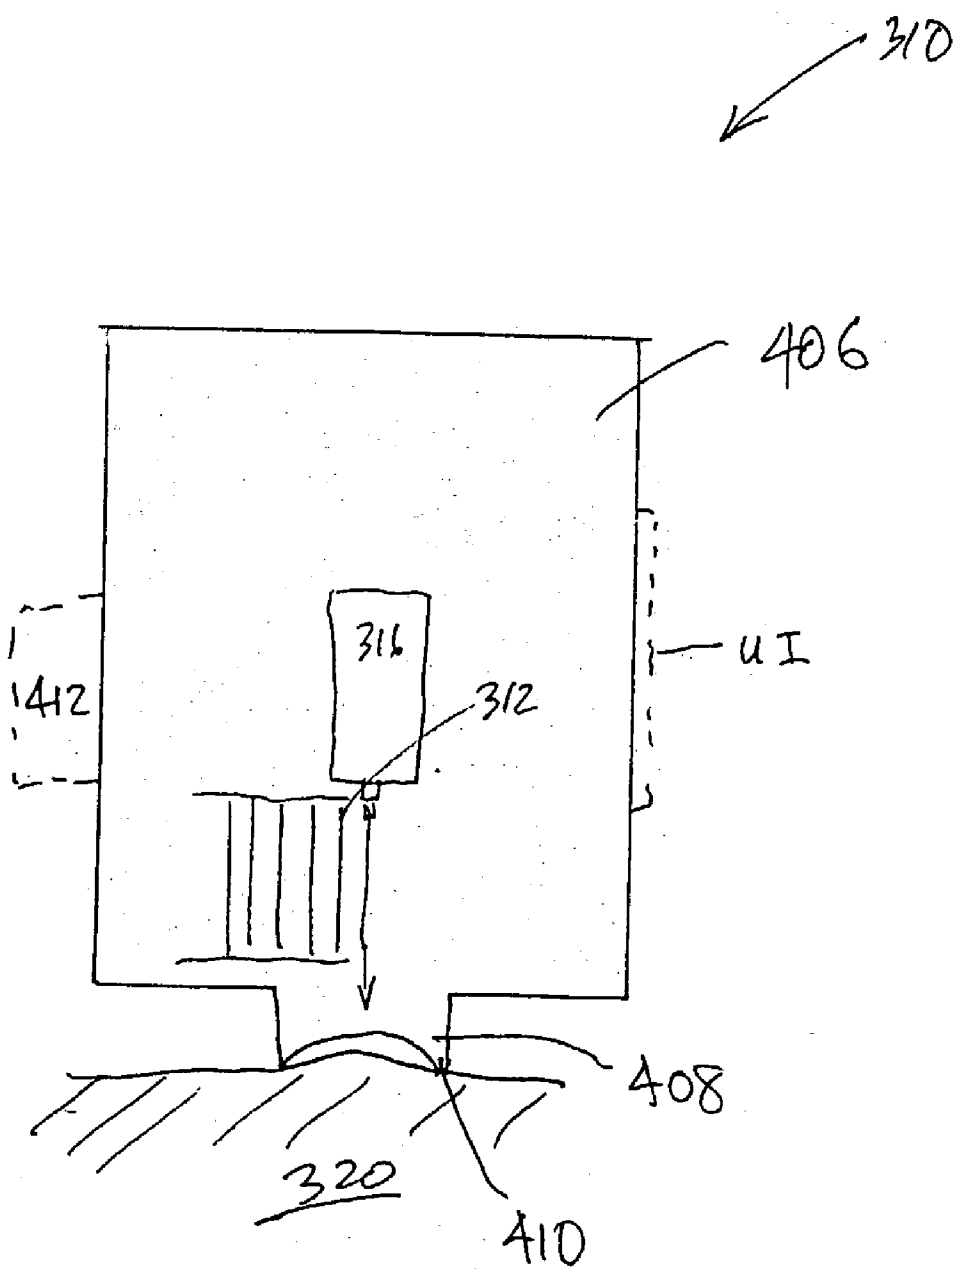


FIG. 35


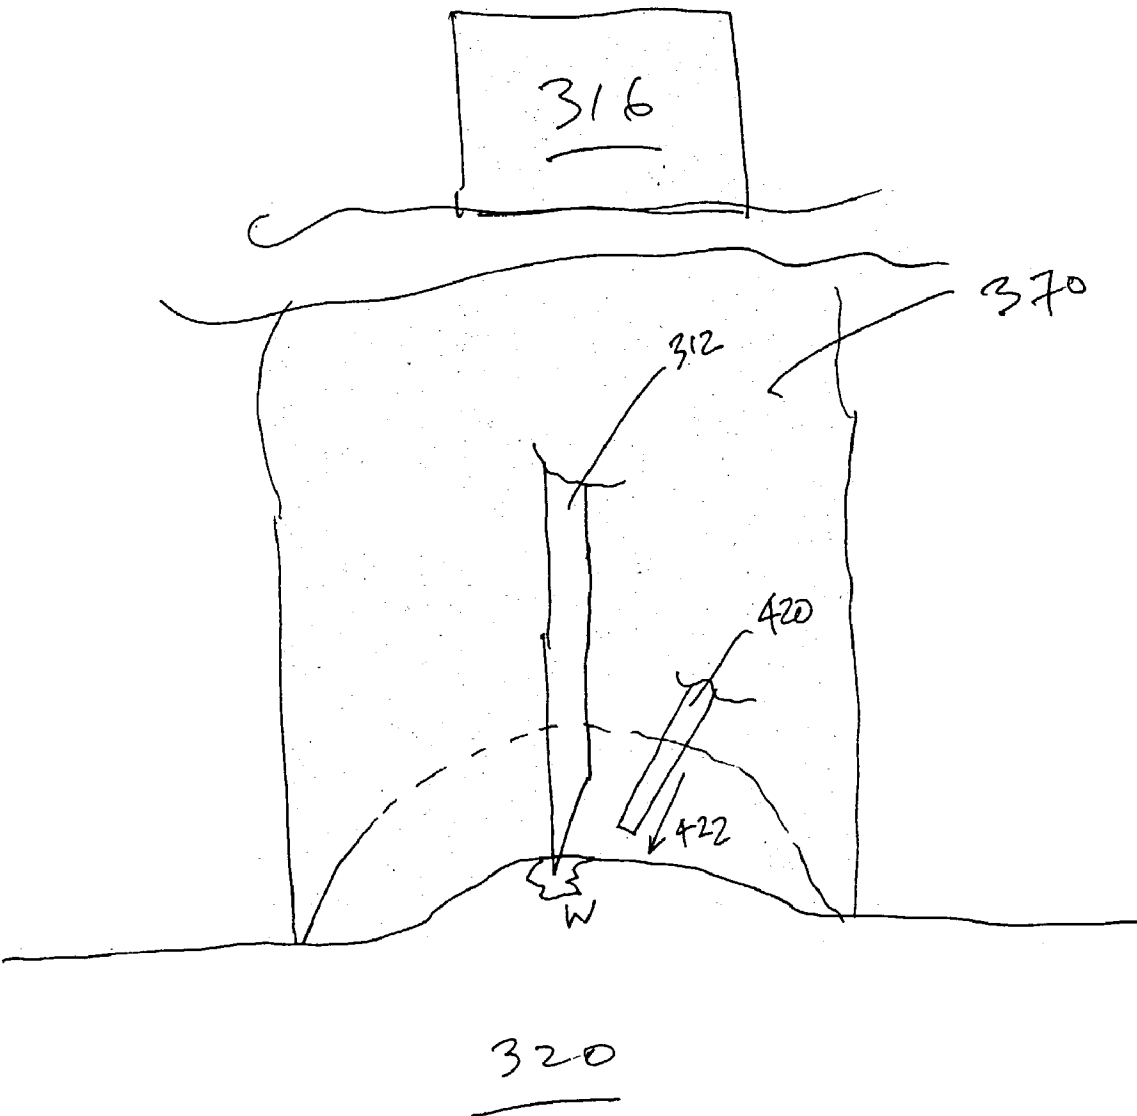


FIG - 36

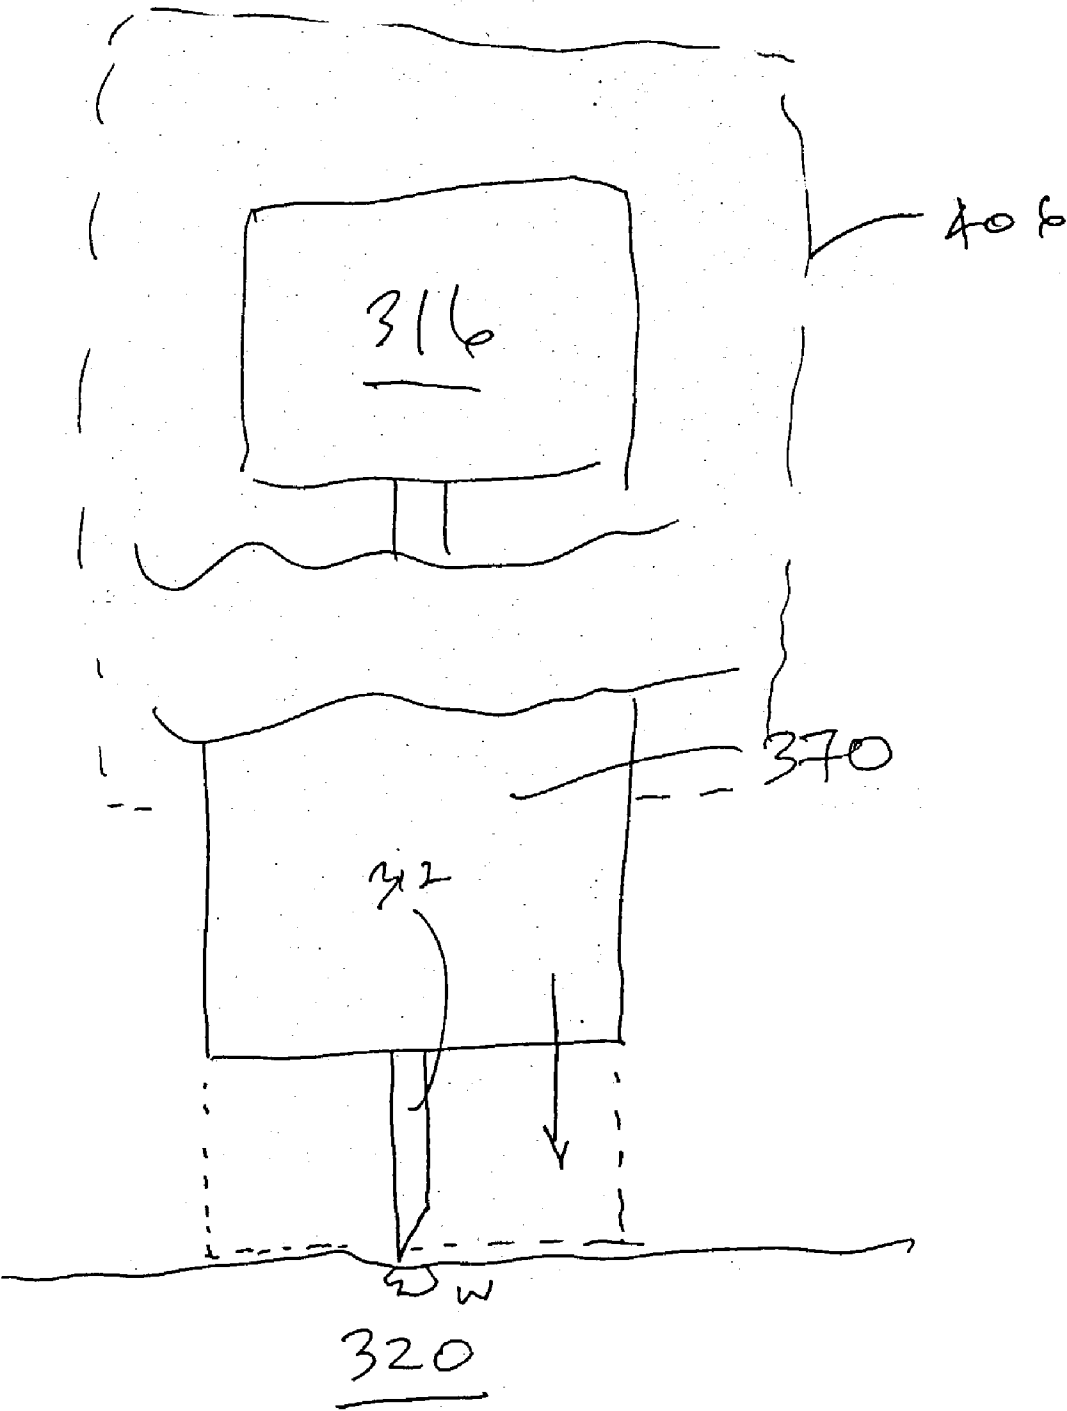

FIG\_37

## METHOD AND APPARATUS FOR PENETRATING TISSUE

### CROSS REFERENCE TO RELATED APPLICATION

[0001] This application is a continuation-in-part of commonly assigned, copending U.S. patent application Ser. No. 10/127,395 (Attorney Docket No. 38187-2551) filed Apr. 19, 2002. This application also claims the benefit of priority from commonly assigned, copending U.S. patent application Ser. No. 10/237,261 (Attorney Docket No. 38187-2595) filed Sep. 5, 2002 and commonly assigned, copending U.S. patent application Ser. No. 10/\_\_\_\_\_ (Attorney Docket No. 38187-2592) filed Sep. 5, 2002. All applications listed above are fully incorporated herein by reference for all purposes.

### BACKGROUND OF THE INVENTION

[0002] Lancing devices are known in the medical health-care products industry for piercing the skin to produce blood for analysis. Typically, a drop of blood for this type of analysis is obtained by making a small incision in the fingertip, creating a small wound, which generates a small blood droplet on the surface of the skin.

[0003] Early methods of lancing included piercing or slicing the skin with a needle or razor. Current methods utilize lancing devices that contain a multitude of spring, cam and mass actuators to drive the lancet. These include cantilever springs, diaphragms, coil springs, as well as gravity plumbs used to drive the lancet. The device may be held against the skin and mechanically triggered to ballistically launch the lancet. Unfortunately, the pain associated with each lancing event using known technology discourages patients from testing. In addition to vibratory stimulation of the skin as the driver impacts the end of a launcher stop, known spring based devices have the possibility of harmonically oscillating against the patient tissue, causing multiple strikes due to recoil. This recoil and multiple strikes of the lancet against the patient is one major impediment to patient compliance with a structured glucose monitoring regime.

[0004] Another impediment to patient compliance is the lack of spontaneous blood flow generated by known lancing technology. In addition to the pain as discussed above, a patient may need more than one lancing event to obtain a blood sample since spontaneous blood generation is unreliable using known lancing technology. Thus the pain is multiplied by the number of tries it takes to successfully generate spontaneous blood flow. Different skin thickness may yield different results in terms of pain perception, blood yield and success rate of obtaining blood between different users of the lancing device. Known devices poorly account for these skin thickness variations.

[0005] A still further impediment to improved compliance with glucose monitoring are the many steps and hassle associated with each lancing event. Many diabetic patients that are insulin dependent may need to self-test for blood glucose levels five to six times daily. The large number of steps required in traditional methods of glucose testing, ranging from lancing, to milking of blood, applying blood to the test strip, and getting the measurements from the test strip, discourages many diabetic patients from testing their blood glucose levels as often as recommended. Older

patients and those with deteriorating motor skills encounter difficulty loading lancets into launcher devices, transferring blood onto a test strip, or inserting thin test strips into slots on glucose measurement meters. Additionally, the wound channel left on the patient by known systems may also be of a size that discourages those who are active with their hands or who are worried about healing of those wound channels from testing their glucose levels.

### SUMMARY OF THE INVENTION

[0006] Accordingly, an object of the present invention is to provide improved tissue penetrating systems, and their methods of use.

[0007] Another object of the present invention is to provide tissue penetrating systems, and their methods of use, that provide reduced pain when penetrating a target tissue.

[0008] Yet another object of the present invention is to provide tissue penetrating systems, and their methods of use, that provide controlled depth of penetration.

[0009] Still a further object of the present invention is to provide tissue penetrating systems, and their methods of use, that provide controlled velocities into and out of target tissue.

[0010] A further object of the present invention is to provide tissue penetrating systems, and their methods of use, that provide stimulation to a target tissue.

[0011] Another object of the present invention is to provide tissue penetrating systems, and their methods of use, that apply a pressure to a target tissue.

[0012] Yet another object of the present invention is to provide tissue penetrating systems, and their methods of use, with penetrating members that remain in sterile environments prior to launch.

[0013] Still another object of the present invention is to provide tissue penetrating systems, and their methods of use, with penetrating members that remain in sterile environments prior to launch, and the penetrating members are not used to breach the sterile environment.

[0014] A further object of the present invention is to provide improved tissue penetrating systems, and their methods of use, that have user interfaces.

[0015] Another object of the present invention is to provide improved tissue penetrating systems, and their methods of use, that have human interfaces.

[0016] Yet another object of the present invention is to provide tissue penetrating systems, and their methods of use, that have low volume sample chambers.

[0017] Still another object of the present invention is to provide tissue penetrating systems, and their methods of use, that have sample chambers with volumes that do not exceed 1  $\mu$ L.

[0018] Another object of the present invention is to provide tissue penetrating systems, and their methods of use, that have multiple penetrating members housed in a cartridge.

[0019] In one embodiment of the present invention, a tissue penetration device includes a penetrating member

driver and a cartridge. A plurality of penetrating members are integrated with the cartridge. Each penetrating member is coupled to the penetrating member driver when advanced along a path into a tissue target. A penetrating member sensor is coupled to the plurality of penetrating members. The penetrating member sensor is configured to provide information relative to a depth of penetration of a penetrating member through a skin surface.

[0020] In another embodiment of the present invention, a tissue penetrating system includes a plurality of penetrating members coupled to a penetrating member driver. A cartridge transport device is included. A plurality of cartridges are provided, each being associated with a penetrating member. The cartridge transport device is configured to move each cartridge to a position aligning a penetrating member with the penetrating member driver to drive the penetrating member along a path into a target tissue site.

[0021] In another embodiment of the present invention, a tissue penetrating device includes a penetrating member. A penetrating member driver is coupled to the penetrating member. A penetrating member sensor is coupled to the penetrating member. The penetrating member sensor is configured to provide information relative to a depth of penetration of a penetrating member through a skin surface. A processor is coupled to the penetrating member sensor. The processor produces a signal indicative of a change in direction and magnitude of force exerted on the penetrating member. The processor is further configured to cause application of a braking force to the penetrating member.

[0022] In another embodiment of the present invention, a skin penetrating device includes a penetrating member driver. A penetrating member is coupled to the penetrating member driver. A damper is coupled to the penetrating member driver for preventing multiple oscillations of the penetrating member in the tissue target once the penetrating member has reached a desired depth.

[0023] In another embodiment of the present invention, a method of penetrating a target tissue advances a penetrating member through the target tissue. The penetrating member is stopped at a desired depth below a skin surface without multiple oscillations against the skin surface. The penetrating member is withdrawn from the target tissue.

[0024] In another embodiment of the present invention, a method of penetrating a target tissue provides a tissue penetrating system that includes a penetrating member driver, a plurality of cartridges, a plurality of penetrating members each associated with a cartridge, a plurality of sample chambers each associated with a penetrating member, and a penetrating member sensor. A penetrating member is advanced from a cartridge into the target tissue. The penetrating member is withdrawn from the target tissue. An analyte sample is received in a sample chamber.

[0025] A further understanding of the nature and advantages of the invention will become apparent by reference to the remaining portions of the specification and drawings.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0026] FIG. 1 illustrates an embodiment of a controllable force driver in the form of a cylindrical electric penetrating member driver using a coiled solenoid-type configuration.

[0027] FIG. 2A illustrates a displacement over time profile of a penetrating member driven by a harmonic spring/mass system.

[0028] FIG. 2B illustrates the velocity over time profile of a penetrating member driver by a harmonic spring/mass system.

[0029] FIG. 2C illustrates a displacement over time profile of an embodiment of a controllable force driver.

[0030] FIG. 2D illustrates a velocity over time profile of an embodiment of a controllable force driver.

[0031] FIG. 3 is a diagrammatic view illustrating a controlled feed-back loop.

[0032] FIG. 4 is a perspective view of a tissue penetration device having features of the invention.

[0033] FIG. 5 is an elevation view in partial longitudinal section of the tissue penetration device of FIG. 4.

[0034] FIGS. 6A-6C show a flowchart illustrating a penetrating member control method.

[0035] FIG. 7 is a diagrammatic view of a patient's finger and a penetrating member tip moving toward the skin of the finger.

[0036] FIG. 8 is a diagrammatic view of a patient's finger and the penetrating member tip making contact with the skin of a patient's finger.

[0037] FIG. 9 is a diagrammatic view of the penetrating member tip depressing the skin of a patient's finger.

[0038] FIG. 10 is a diagrammatic view of the penetrating member tip further depressing the skin of a patient's finger.

[0039] FIG. 11 is a diagrammatic view of the penetrating member tip penetrating the skin of a patient's finger.

[0040] FIG. 12 is a diagrammatic view of the penetrating member tip penetrating the skin of a patient's finger to a desired depth.

[0041] FIG. 13 is a diagrammatic view of the penetrating member tip withdrawing from the skin of a patient's finger.

[0042] FIGS. 14-18 illustrate a method of tissue penetration that may measure elastic recoil of the skin.

[0043] FIG. 19 is a perspective view in partial section of a tissue penetration sampling device with a cartridge of sampling modules.

[0044] FIG. 20 is a perspective view of a sampling module cartridge with the sampling modules arranged in a ring configuration.

[0045] FIG. 21 illustrate an embodiment of a cartridge for use in sampling having a sampling cartridge body and a penetrating member cartridge body.

[0046] FIG. 22A shows a device for use on a tissue site having a plurality of penetrating members.

[0047] FIG. 22B shows rear view of a device for use on a tissue site having a plurality of penetrating members.

[0048] FIG. 22C shows a schematic of a device for use on a tissue site with a feedback loop and optionally a damper.

[0049] FIG. 23A shows an embodiment of a device with a user interface.

[0050] FIG. 23B shows an outer view of a device with a user interface.

[0051] FIG. 24 is a cut away view of a system for sampling body fluid.

[0052] FIG. 25 is an exploded view of a cartridge for use with a system for sampling body fluid.

[0053] FIG. 26 is an exploded view of a cartridge having multiple penetrating members for use with a system for sampling body fluid.

[0054] FIGS. 27-28 show cartridges for use with a system for sampling body fluid.

[0055] FIG. 29 shows a cutaway view of another embodiment of a system for sampling body fluid.

[0056] FIG. 30 shows the density associated with a cartridge according to the present invention.

[0057] FIG. 31 shows a cutaway view of another embodiment of a system for sampling body fluid.

[0058] FIG. 32 is a cut away view of a cartridge according to the present invention.

[0059] FIGS. 33-34 show views of a body sampling system using multiple cartridges.

[0060] FIG. 35 shows an embodiment of the present invention with a tissue stabilizing member.

[0061] FIG. 36 shows a cartridge according to the present invention with a tissue stabilizing member.

[0062] FIG. 37 shows a system according to the present invention with a moveable cartridge.

#### DESCRIPTION OF THE SPECIFIC EMBODIMENTS

[0063] The present invention provides a solution for body fluid sampling. Specifically, some embodiments of the present invention provides a penetrating member device for consistently creating a wound with spontaneous body fluid flow from a patient. The invention may be a multiple penetrating member device with an optional high density design. It may use penetrating members of smaller size than known penetrating members. The device may be used for multiple lancing events without having to remove a disposable from the device or for the user to handle sharps. The invention may provide improved sensing capabilities. At least some of these and other objectives described herein will be met by embodiments of the present invention.

[0064] It is to be understood that both the foregoing general description and the following detailed description are exemplary and explanatory only and are not restrictive of the invention, as claimed. It should be noted that, as used in the specification and the appended claims, the singular forms "a", "an" and "the" include plural referents unless the context clearly dictates otherwise. Thus, for example, reference to "a material" may include mixtures of materials, reference to "a chamber" may include multiple chambers, and the like. References cited herein are hereby incorporated

by reference in their entirety, except to the extent that they conflict with teachings explicitly set forth in this specification.

[0065] In this specification and in the claims which follow, reference will be made to a number of terms which shall be defined to have the following meanings:

[0066] "Optional" or "optionally" means that the subsequently described circumstance may or may not occur, so that the description includes instances where the circumstance occurs and instances where it does not. For example, if a device optionally contains a feature for analyzing a blood sample, this means that the analysis feature may or may not be present, and, thus, the description includes structures wherein a device possesses the analysis feature and structures wherein the analysis feature is not present.

[0067] "Analyte detecting member" refers to any use, singly or in combination, of chemical test reagents and methods, electrical test circuits and methods, physical test components and methods, optical test components and methods, and biological test reagents and methods to yield information about a blood sample. Such methods are well known in the art and may be based on teachings of, e.g. Tietz Textbook of Clinical Chemistry, 3d Ed., Sec. V, pp. 776-78 (Burtis & Ashwood, Eds., W. B. Saunders Company, Philadelphia, 1999); U.S. Pat. No. 5,997,817 to Chrismore et al. (Dec. 7, 1999); U.S. Pat. No. 5,059,394 to Phillips et al. (Oct. 22, 1991); U.S. Pat. No. 5,001,054 to Wagner et al. (Mar. 19, 1991); and U.S. Pat. No. 4,392,933 to Nakamura et al. (Jul. 12, 1983), the teachings of which are hereby incorporated by reference, as well as others. Analyte detecting member may include tests in the sample test chamber that test electrochemical properties of the blood, or they may include optical means for sensing optical properties of the blood (e.g. oxygen saturation level), or they may include biochemical reagents (e.g. antibodies) to sense properties (e.g. presence of antigens) of the blood. The analyte detecting member may comprise biosensing or reagent material that will react with an analyte in blood (e.g. glucose) or other body fluid so that an appropriate signal correlating with the presence of the analyte is generated and can be read by the reader apparatus. By way of example and not limitation, analyte detecting member may "associated with", "mounted within", or "coupled to" a chamber or other structure when the analyte detecting member participates in the function of providing an appropriate signal about the blood sample to the reader device. Analyte detecting member may also include nanowire analyte detecting members as described herein. Analyte detecting member may use potentiometric, coulometric, or other method useful for detection of analyte levels.

[0068] The present invention may be used with a variety of different penetrating member drivers. It is contemplated that these penetrating member drivers may be spring based, solenoid based, magnetic driver based, nanomuscle based, or based on any other mechanism useful in moving a penetrating member along a path into tissue. It should be noted that the present invention is not limited by the type of driver used with the penetrating member feed mechanism. One suitable penetrating member driver for use with the present invention is shown in FIG. 1. This is an embodiment of a solenoid type electromagnetic driver that is capable of driving an iron core or slug mounted to the penetrating

member assembly using a direct current (DC) power supply. The electromagnetic driver includes a driver coil pack that is divided into three separate coils along the path of the penetrating member, two end coils and a middle coil. Direct current is alternated to the coils to advance and retract the penetrating member. Although the driver coil pack is shown with three coils, any suitable number of coils may be used, for example, 4, 5, 6, 7 or more coils may be used.

**[0069]** Referring to the embodiment of **FIG. 1**, the stationary iron housing **10** may contain the driver coil pack with a first coil **12** flanked by iron spacers **14** which concentrate the magnetic flux at the inner diameter creating magnetic poles. The inner insulating housing **16** isolates the penetrating member **18** and iron core **20** from the coils and provides a smooth, low friction guide surface. The penetrating member guide **22** further centers the penetrating member **18** and iron core **20**. The penetrating member **18** is protracted and retracted by alternating the current between the first coil **12**, the middle coil, and the third coil to attract the iron core **20**. Reversing the coil sequence and attracting the core and penetrating member back into the housing retracts the penetrating member. The penetrating member guide **22** also serves as a stop for the iron core **20** mounted to the penetrating member **18**.

**[0070]** As discussed above, tissue penetration devices which employ spring or cam driving methods have a symmetrical or nearly symmetrical actuation displacement and velocity profiles on the advancement and retraction of the penetrating member as shown in **FIGS. 2 and 3**. In most of the available lancet devices, once the launch is initiated, the stored energy determines the velocity profile until the energy is dissipated. Controlling impact, retraction velocity, and dwell time of the penetrating member within the tissue can be useful in order to achieve a high success rate while accommodating variations in skin properties and minimize pain. Advantages can be achieved by taking into account of the fact that tissue dwell time is related to the amount of skin deformation as the penetrating member tries to puncture the surface of the skin and variance in skin deformation from patient to patient based on skin hydration.

**[0071]** In this embodiment, the ability to control velocity and depth of penetration may be achieved by use of a controllable force driver where feedback is an integral part of driver control. Such drivers can control either metal or polymeric penetrating members or any other type of tissue penetration element. The dynamic control of such a driver is illustrated in **FIG. 2C** which illustrates an embodiment of a controlled displacement profile and **FIG. 2D** which illustrates an embodiment of a controlled velocity profile. These are compared to **FIGS. 2A and 2B**, which illustrate embodiments of displacement and velocity profiles, respectively, of a harmonic spring/mass powered driver. Reduced pain can be achieved by using impact velocities of greater than about 2 m/s entry of a tissue penetrating element, such as a lancet, into tissue. Other suitable embodiments of the penetrating member driver are described in commonly assigned, copending U.S. patent application Ser. No. 10/127,395, (Attorney Docket No. 38187-2551) filed Apr. 19, 2002 and previously incorporated herein.

**[0072]** **FIG. 3** illustrates the operation of a feedback loop using a processor **60**. The processor **60** stores profiles **62** in non-volatile memory. A user inputs information **64** about the

desired circumstances or parameters for a lancing event. The processor **60** selects a driver profile **62** from a set of alternative driver profiles that have been preprogrammed in the processor **60** based on typical or desired tissue penetration device performance determined through testing at the factory or as programmed in by the operator. The processor **60** may customize by either scaling or modifying the profile based on additional user input information **64**. Once the processor has chosen and customized the profile, the processor **60** is ready to modulate the power from the power supply **66** to the penetrating member driver **68** through an amplifier **70**. The processor **60** may measure the location of the penetrating member **72** using a position sensing mechanism **74** through an analog to digital converter **76** linear encoder or other such transducer. Examples of position sensing mechanisms have been described in the embodiments above and may be found in the specification for commonly assigned, copending U.S. patent application Ser. No. 10/127,395, (Attorney Docket No. 38187-2551) filed Apr. 19, 2002 and previously incorporated herein. The processor **60** calculates the movement of the penetrating member by comparing the **20** actual profile of the penetrating member to the predetermined profile. The processor **60** modulates the power to the penetrating member driver **68** through a signal generator **78**, which may control the amplifier **70** so that the actual velocity profile of the penetrating member does not exceed the predetermined profile by more than a preset error limit. The error limit is the accuracy in the control of the penetrating member.

**[0073]** After the lancing event, the processor **60** can allow the user to rank the results of the lancing event. The processor **60** stores these results and constructs a database **80** for the individual user. Using the database **79**, the processor **60** calculates the profile traits such as degree of painlessness, success rate, and blood volume for various profiles **62** depending on user input information **64** to optimize the profile to the individual user for subsequent lancing cycles. **30** These profile traits depend on the characteristic phases of penetrating member advancement and retraction. The processor **60** uses these calculations to optimize profiles **62** for each user. In addition to user input information **64**, an internal clock allows storage in the database **79** of information such as the time of day to generate a time stamp for the lancing event and the time between lancing events to anticipate the user's diurnal needs. The database stores information and statistics for each user and each profile that particular user uses.

**[0074]** In addition to varying the profiles, the processor **60** can be used to calculate the appropriate penetrating member diameter and geometry suitable to realize the blood volume required by the user. For example, if the user requires about 1-5 microliter volume of blood, the processor **60** may select a 200 micron diameter penetrating member to achieve these results. For each class of lancet, both diameter and lancet tip geometry, is stored in the processor **60** to correspond with upper and lower limits of attainable blood volume based on the predetermined displacement and velocity profiles.

**[0075]** The lancing device is capable of prompting the user for information at the beginning and the end of the lancing event to more adequately suit the user. The goal is to either change to a different profile or modify an existing profile. Once the profile is set, the force driving the penetrating member is varied during advancement and retraction to

follow the profile. The method of lancing using the lancing device comprises selecting a profile, lancing according to the selected profile, determining lancing profile traits for each characteristic phase of the lancing cycle, and optimizing profile traits for subsequent lancing events.

[0076] FIG. 4 illustrates an embodiment of a tissue penetration device, more specifically, a lancing device 80 that includes a controllable driver 179 coupled to a tissue penetration element. The lancing device 80 has a proximal end 81 and a distal end 82. At the distal end 82 is the tissue penetration element in the form of a penetrating member 83, which is coupled to an elongate coupler shaft 84 by a drive coupler 85. The elongate coupler shaft 84 has a proximal end 86 and a distal end 87. A driver coil pack 88 is disposed about the elongate coupler shaft 84 proximal of the penetrating member 83. A position sensor 91 is disposed about a proximal portion 92 of the elongate coupler shaft 84 and an electrical conductor 94 electrically couples a processor 93 to the position sensor 91. The elongate coupler shaft 84 driven by the driver coil pack 88 controlled by the position sensor 91 and processor 93 form the controllable driver, specifically, a controllable electromagnetic driver.

[0077] Referring to FIG. 5, the lancing device 80 can be seen in more detail, in partial longitudinal section. The penetrating member 83 has a proximal end 95 and a distal end 96 with a sharpened point at the distal end 96 of the penetrating member 83 and a drive head 98 disposed at the proximal end 95 of the penetrating member 83. A penetrating member shaft 201 is disposed between the drive head 98 and the sharpened point 97. The penetrating member shaft 201 may be comprised of stainless steel, or any other suitable material or alloy and have a transverse dimension of about 0.1 to about 0.4 mm. The penetrating member shaft may have a length of about 3 mm to about 50 mm, specifically, about 15 mm to about 20 mm. The drive head 98 of the penetrating member 83 is an enlarged portion having a transverse dimension greater than a transverse dimension of the penetrating member shaft 201 distal of the drive head 98. This configuration allows the drive head 98 to be mechanically captured by the drive coupler 85. The drive head 98 may have a transverse dimension of about 0.5 to about 2 mm.

[0078] A magnetic member 102 is secured to the elongate coupler shaft 84 proximal of the drive coupler 85 on a distal portion 203 of the elongate coupler shaft 84. The magnetic member 102 is a substantially cylindrical piece of magnetic material having an axial lumen 204 extending the length of the magnetic member 102. The magnetic member 102 has an outer transverse dimension that allows the magnetic member 102 to slide easily within an axial lumen 105 of a low friction, possibly lubricious, polymer guide tube 105' disposed within the driver coil pack 88. The magnetic member 102 may have an outer transverse dimension of about 1.0 to about 5.0 mm, specifically, about 2.3 to about 2.5 mm. The magnetic member 102 may have a length of about 3.0 to about 5.0 mm, specifically, about 4.7 to about 4.9 mm. The magnetic member 102 can be made from a variety of magnetic materials including ferrous metals such as ferrous steel, iron, ferrite, or the like. The magnetic member 102 may be secured to the distal portion 203 of the elongate coupler shaft 84 by a variety of methods including adhesive or epoxy bonding, welding, crimping or any other suitable method.

[0079] Proximal of the magnetic member 102, an optical encoder flag 206 is secured to the elongate coupler shaft 84. The optical encoder flag 206 is configured to move within a slot 107 in the position sensor 91. The slot 107 of the position sensor 91 is formed between a first body portion 108 and a second body portion 109 of the position sensor 91. The slot 107 may have separation width of about 1.5 to about 2.0 mm. The optical encoder flag 206 can have a length of about 14 to about 18 mm, a width of about 3 to about 5 mm and a thickness of about 0.04 to about 0.06 mm.

[0080] The optical encoder flag 206 interacts with various optical beams generated by LEDs disposed on or in the position sensor body portions 108 and 109 in a predetermined manner. The interaction of the optical beams generated by the LEDs of the position sensor 91 generates a signal that indicates the longitudinal position of the optical flag 206 relative to the position sensor 91 with a substantially high degree of resolution. The resolution of the position sensor 91 may be about 200 to about 400 cycles per inch, specifically, about 350 to about 370 cycles per inch. The position sensor 91 may have a speed response time (position/time resolution) of 0 to about 120,000 Hz, where one dark and light stripe of the flag constitutes one Hertz, or cycle per second. The position of the optical encoder flag 206 relative to the magnetic member 102, driver coil pack 88 and position sensor 91 is such that the optical encoder 91 can provide precise positional information about the penetrating member 83 over the entire length of the penetrating member's power stroke.

[0081] An optical encoder that is suitable for the position sensor 91 is a linear optical incremental encoder, model HEDS 9200, manufactured by Agilent Technologies. The model HEDS 9200 may have a length of about 20 to about 30 mm, a width of about 8 to about 12 mm, and a height of about 9 to about 11 mm. Although the position sensor 91 illustrated is a linear optical incremental encoder, other suitable position sensor embodiments could be used, provided they possess the requisite positional resolution and time response. The HEDS 9200 is a two channel device where the channels are 90 degrees out of phase with each other. This results in a resolution of four times the basic cycle of the flag. These quadrature outputs make it possible for the processor to determine the direction of penetrating member travel. Other suitable position sensors include capacitive encoders, analog reflective sensors, such as the reflective position sensor discussed above, and the like.

[0082] A coupler shaft guide 111 is disposed towards the proximal end 81 of the lancing device 80. The guide 111 has a guide lumen 112 disposed in the guide 111 to slidably accept the proximal portion 92 of the elongate coupler shaft 84. The guide 111 keeps the elongate coupler shaft 84 centered horizontally and vertically in the slot 102 of the optical encoder 91.

[0083] The driver coil pack 88, position sensor 91 and coupler shaft guide 111 are all secured to a base 113. The base 113 is longitudinally coextensive with the driver coil pack 88, position sensor 91 and coupler shaft guide 111. The base 113 can take the form of a rectangular piece of metal or polymer, or may be a more elaborate housing with recesses, which are configured to accept the various components of the lancing device 80.

[0084] As discussed above, the magnetic member 102 is configured to slide within an axial lumen 105 of the driver

coil pack **88**. The driver coil pack **88** includes a most distal first coil **114**, a second coil **115**, which is axially disposed between the first coil **114** and a third coil **116**, and a proximal-most fourth coil **117**. Each of the first coil **114**, second coil **115**, third coil **116** and fourth coil **117** has an axial lumen. The axial lumens of the first through fourth coils are configured to be coaxial with the axial lumens of the other coils and together form the axial lumen **105** of the driver coil pack **88** as a whole. Axially adjacent each of the coils **114-117** is a magnetic disk or washer **118** that augments completion of the magnetic circuit of the coils **114-117** during a lancing cycle of the device **80**. The magnetic washers **118** of the embodiment of **FIG. 5** are made of ferrous steel but could be made of any other suitable magnetic material, such as iron or ferrite. The outer shell **89** of the driver coil pack **88** is also made of iron or steel to complete the magnetic path around the coils and between the washers **118**. The magnetic washers **118** have an outer diameter commensurate with an outer diameter of the driver coil pack **88** of about 4.0 to about 8.0 mm. The magnetic washers **118** have an axial thickness of about 0.05, to about 0.4 mm, specifically, about 0.15 to about 0.25 mm.

**[0085]** Wrapping or winding an elongate electrical conductor **121** about an axial lumen until a sufficient number of windings have been achieved forms the coils **114-117**. The elongate electrical conductor **121** is generally an insulated solid copper wire with a small outer transverse dimension of about 0.06 mm to about 0.88 mm, specifically, about 0.3 mm to about 0.5 mm. In one embodiment, **32** gauge copper wire is used for the coils **114-117**. The number of windings for each of the coils **114-117** of the driver pack **88** may vary with the size of the coil, but for some embodiments each coil **114-117** may have about 30 to about 80 turns, specifically, about 50 to about 60 turns. Each coil **114-117** can have an axial length of about 1.0 to about 3.0 mm, specifically, about 1.8 to about 2.0 mm. Each coil **114-117** can have an outer transverse dimension or diameter of about 4.0, to about 2.0 mm, specifically, about 9.0 to about 12.0 mm. The axial lumen **105** can have a transverse dimension of about 1.0 to about 3.0 mm.

**[0086]** It may be advantageous in some driver coil **88** embodiments to replace one or more of the coils with permanent magnets, which produce a magnetic field similar to that of the coils when the coils are activated. In particular, it may be desirable in some embodiments to replace the second coil **115**, the third coil **116** or both with permanent magnets. In addition, it may be advantageous to position a permanent magnet at or near the proximal end of the coil driver pack in order to provide fixed magnet zeroing function for the magnetic member (Adams magnetic Products 23A0002 flexible magnet material (800) 747-7543).

**[0087]** **FIGS. 20 and 21** show a permanent bar magnet **119** disposed on the proximal end of the driver coil pack **88**. As shown in **FIG. 5**, the bar magnet **119** is arranged so as to have one end disposed adjacent the travel path of the magnetic member **102** and has a polarity configured so as to attract the magnetic member **102** in a centered position with respect to the bar magnet **119**. Note that the polymer guide tube **105'** can be configured to extend proximally to insulate the inward radial surface of the bar magnet **119** from an outer surface of the magnetic member **102**. This arrangement allows the magnetic member **119** and thus the elongate

coupler shaft **84** to be attracted to and held in a zero point or rest position without the consumption of electrical energy from the power supply **125**.

**[0088]** Having a fixed zero or start point for the elongate coupler shaft **84** and penetrating member **83** may be useful to properly controlling the depth of penetration of the penetrating member **83** as well as other lancing parameters. This can be because some methods of depth penetration control for a controllable driver measure the acceleration and displacement of the elongate coupler shaft **84** and penetrating member **83** from a known start position. If the distance of the penetrating member tip **96** from the target tissue is known, acceleration and displacement of the penetrating member is known and the start position of the penetrating member is known, the time and position of tissue contact and depth of penetration can be determined by the processor **93**.

**[0089]** Any number of configurations for a magnetic bar **119** can be used for the purposes discussed above. In particular, a second permanent bar magnet (not shown) could be added to the proximal end of the driver coil pack **88** with the magnetic fields of the two bar magnets configured to complement each other. In addition, a disc magnet **119'** could be used as illustrated in **FIG. 22**. Disc magnet **119'** is shown disposed at the proximal end of the driver coiled pack **88** with a polymer non-magnetic disc **119''** disposed between the proximal-most coil **117** and disc magnet **119'** and positions disc magnet **119'** away from the proximal end of the proximal-most coil **117**. The polymer non-magnetic disc spacer **119''** is used so that the magnetic member **102** can be centered in a zero or start position slightly proximal of the proximal-most coil **117** of the driver coil pack **88**. This allows the magnetic member to be attracted by the proximal-most coil **117** at the initiation of the lancing cycle instead of being passive in the forward drive portion of the lancing cycle.

**[0090]** An inner lumen of the polymer non-magnetic disc **119''** can be configured to allow the magnetic member **102** to pass axially there through while an inner lumen of the disc magnet **119'** can be configured to allow the elongate coupler shaft **84** to pass through but not large enough for the magnetic member **102** to pass through. This results in the magnetic member **102** being attracted to the disc magnet **119'** and coming to rest with the proximal surface of the magnetic member **102** against a distal surface of the disc magnet **119'**. This arrangement provides for a positive and repeatable stop for the magnetic member, and hence the penetrating member. A similar configuration could also be used for the bar magnet **119** discussed above.

**[0091]** Typically, when the electrical current in the coils **114-117** of the driver coil pack **88** is off, a magnetic member **102** made of soft iron is attracted to the bar magnet **119** or disc magnet **119'**. The magnetic field of the driver coil pack **88** and the bar magnet **119** or disc magnet **119'**, or any other suitable magnet, can be configured such that when the electrical current in the coils **114-117** is turned on, the leakage magnetic field from the coils **114-117** has the same polarity as the bar magnet **119** or disc magnet **119'**. This results in a magnetic force that repels the magnetic member **102** from the bar magnet **119** or disc magnet **119'** and attracts the magnetic member **102** to the activated coils **114-117**. For this configuration, the bar magnet **119** or disc magnet thus

act to facilitate acceleration of the magnetic member 102 as opposed to working against the acceleration.

[0092] Electrical conductors 122 couple the driver coil pack 88 with the processor 93 which can be configured or programmed to control the current flow in the coils 114-117 of the driver coil pack 88 based on position feedback from the position sensor 91, which is coupled to the processor 93 by electrical conductors 94. A power source 125 is electrically coupled to the processor 93 and provides electrical power to operate the processor 93 and power the coil driver pack 88. The power source 125 may be one or more batteries that provide direct current power to the 93 processor.

[0093] Referring to FIGS. 29A-29C, a flow diagram is shown that describes the operations performed by the processor 93 in controlling the penetrating member 83 of the lancing device 80 discussed above during an operating cycle. FIGS. 30-36 illustrate the interaction of the penetrating member 83 and skin 133 of the patient's finger 134 during an operation cycle of the penetrating member device 83. The processor 93 operates under control of programming steps that are stored in an associated memory. When the programming steps are executed, the processor 93 performs operations as described herein. Thus, the programming steps implement the functionality of the operations described with respect to the flow , diagram of FIG. 29. The processor 93 can receive the programming steps from a program product stored in recordable media, including a direct access program product storage device such as a hard drive or flash ROM, a removable program product storage device such as a floppy disk, or in any other manner known to those of skill in the art. The processor 93 can also download the programming steps through a network connection or serial connection.

[0094] In the first operation, represented by the flow diagram box numbered 245 in FIG. 6A, the processor 93 initializes values that it stores in memory relating to control of the penetrating member, such as variables that it uses to keep track of the controllable driver 179 during movement. For example, the processor may set a clock value to zero and a penetrating member position value to zero or to some other initial value. The processor 93 may also cause power to be removed from the coil pack 88 for a period of time, such as for about 10 ms, to allow any residual flux to dissipate from the coils.

[0095] In the initialization operation, the processor 93 also causes the penetrating member to assume an initial stationary position. When in the initial stationary position, the penetrating member 83 is typically fully retracted such that the magnetic member 102 is positioned substantially adjacent the fourth coil 117 of the driver coil pack 88, shown in FIG. 5 above. The processor 93 can move the penetrating member 83 to the initial stationary position by pulsing an electrical current to the fourth coil 117 to thereby attract the magnetic member 102 on the penetrating member 83 to the fourth coil 117. Alternatively, the magnetic member can be positioned in the initial stationary position by virtue of a permanent magnet, such as bar magnet 119, disc magnet 119' or any other suitable magnet as discussed above with regard to the tissue penetration device illustrated in FIGS. 20 and 21.

[0096] In the next operation, represented by the flow diagram box numbered 247, the processor 93 energizes one

or more of the coils in the coil pack 88. This should cause the penetrating member 83 to begin to move (i.e., achieve a non-zero speed) toward the skin target 133. The processor 93 then determines whether or not the penetrating member is indeed moving, as represented by the decision box numbered 149. The processor 93 can determine whether the penetrating member 83 is moving by monitoring the position of the penetrating member 83 to determine whether the position changes over time. The processor 93 can monitor the position of the penetrating member 83 by keeping track of the position of the optical encoder flag 106 secured to the elongate coupler shaft 84 wherein the encoder 91 produces a signal coupled to the processor 93 that indicates the spatial position of the penetrating member 83.

[0097] If the processor 93 determines (via timeout without motion events) that the penetrating member 83 is not moving (a "No" result from the decision box 149), then the process proceeds to the operation represented by the flow diagram box numbered 153, where the processor deems that an error condition is present. This means that some error in the system is causing the penetrating member 83 not to move. The error may be mechanical, electrical, or software related. For example, the penetrating member 83 may be stuck in the stationary position because something is impeding its movement.

[0098] If the processor 93 determines that the penetrating member 83 is indeed moving (a "Yes" result from the decision box numbered 249), then the process proceeds to the operation represented by the flow diagram box numbered 257. In this operation, the processor 93 causes the penetrating member 83 to continue to accelerate and launch toward the skin target 133, as indicated by the arrow 135 in FIG. 7. The processor 93 can achieve acceleration of the penetrating member 83 by sending an electrical current to an appropriate coil 114-117 such that the coil 114-117 exerts an attractive magnetic launching force on the magnetic member 102 and causes the magnetic member 102 and the penetrating member 83 coupled thereto to move in a desired direction. For example, the processor 93 can cause an electrical current to be sent to the third coil 116 so that the third coil 116 attracts the magnetic member 102 and causes the magnetic member 102 to move from a position adjacent the fourth coil 117 toward the third coil 116. The processor preferably determines which coil 114-117 should be used to attract the magnetic member 102 based on the position of the magnetic member 102 relative to the coils 114-117. In this manner, the processor 93 provides a controlled force to the penetrating member that controls the movement of the penetrating member.

[0099] During this operation, the processor 93 periodically or continually monitors the position and/or velocity of the penetrating member 83. In keeping track of the velocity and position of the penetrating member 83 as the penetrating member 83 moves towards the patient's skin 133 or other tissue, the processor 93 also monitors and adjusts the electrical current to the coils 114-117. In some embodiments, the processor 93 applies current to an appropriate coil 114-117 such that the penetrating member 83 continues to move according to a desired direction and acceleration. In the instant case, the processor 93 applies current to the appropriate coil 114-117 that will cause the penetrating member 83 to continue to move in the direction of the patient's skin 133 or other tissue to be penetrated.

[0100] The processor 93 may successively transition the current between coils 114-117 so that as the magnetic member 102 moves past a particular coil 114-117, the processor 93 then shuts off current to that coil 114-117 and then applies current to another coil 114-117 that will attract the magnetic member 102 and cause the magnetic member 102 to continue to move in the desired direction. In transitioning current between the coils 114-117, the processor 93 can take into account various factors, including the speed of the penetrating member 83, the position of the penetrating member 83 relative to the coils 114-117, the number of coils 114-117, and the level of current to be applied to the coils 114-117 to achieve a desired speed or acceleration.

[0101] In the next operation, the processor 93 determines whether the cutting or distal end tip 96 of the penetrating member 83 has contacted the patient's skin 133, as shown in FIG. 8 and as represented by the decision box numbered 165 in FIG. 6B. The processor 93 may determine whether the penetrating member 83 has made contact with the target tissue 133 by a variety of methods, including some that rely on parameters which are measured prior to initiation of a lancing cycle and other methods that are adaptable to use during a lancing cycle without any predetermined parameters.

[0102] In one embodiment, the processor 93 determines that the skin has been contacted when the end tip 96 of the penetrating member 83 has moved a predetermined distance with respect to its initial position. If the distance from the tip 261 of the penetrating member 83 to the target tissue 133 is known prior to initiation of penetrating member 83 movement, the initial position of the penetrating member 83 is fixed and known, and the movement and position of the penetrating member 83 can be accurately measured during a lancing cycle, then the position and time of penetrating member contact can be determined.

[0103] This method requires an accurate measurement of the distance between the penetrating member tip 96 and the patient's skin 133 when the penetrating member 83 is in the zero time or initial position. This can be accomplished in a number of ways. One way is to control all of the mechanical parameters that influence the distance from the penetrating member tip 96 to the patient's tissue or a surface of the lancing device 80 that will contact the patient's skin 133. This could include the start position of the magnetic member 102, magnetic path tolerance, magnetic member 102 dimensions, driver coil pack 88 location within the lancing device 80 as a whole, length of the elongate coupling shaft 84, placement of the magnetic member 102 on the elongate coupling shaft 84, length of the penetrating member 83 etc.

[0104] If all these parameters, as well as others can be suitably controlled in manufacturing with a tolerance stack-up that is acceptable, then the distance from the penetrating member tip 96 to the target tissue 133 can be determined at the time of manufacture of the lancing device 80. The distance could then be programmed into the memory of the processor 93. If an adjustable feature is added to the lancing device 80, such as an adjustable length elongate coupling shaft 84, this can accommodate variations in all of the parameters noted above, except length of the penetrating member 83. An electronic alternative to this mechanical approach would be to calibrate a stored memory contact point into the memory of the processor 93 during manufacture based on the mechanical parameters described above.

[0105] In another embodiment, moving the penetrating member tip 96 to the target tissue 133 very slowly and gently touching the skin 133 prior to actuation can accomplish the distance from the penetrating member tip 96 to the tissue 133. The position sensor can accurately measure the distance from the initialization point to the point of contact, where the resistance to advancement of the penetrating member 83 stops the penetrating member movement. The penetrating member 83 is then retracted to the initialization point having measured the distance to the target tissue 133 without creating any discomfort to the user.

[0106] In another embodiment, the processor 93 may use software to determine whether the penetrating member 83 has made contact with the patient's skin 133 by measuring for a sudden reduction in velocity of the penetrating member 83 due to friction or resistance imposed on the penetrating member 83 by the patient's skin 133. The optical encoder 91 measures displacement of the penetrating member 83. The position output data provides input to the interrupt input of the processor 93. The processor 93 also has a timer capable of measuring the time between interrupts. The distance between interrupts is known for the optical encoder 91, so the velocity of the penetrating member 83 can be calculated by dividing the distance between interrupts by the time between the interrupts.

[0107] This method requires that velocity losses to the penetrating member 83 and elongate coupler 84 assembly due to friction are known to an acceptable level so that these velocity losses and resulting deceleration can be accounted for when establishing a deceleration threshold above which contact between penetrating member tip 96 and target tissue 133 will be presumed. This same concept can be implemented in many ways. For example, rather than monitoring the velocity of the penetrating member 83, if the processor 93 is controlling the penetrating member driver in order to maintain a fixed velocity, the power, to the driver 88 could be monitored. If an amount of power above a predetermined threshold is required in order to maintain a constant velocity, then contact between the tip of the penetrating member 96 and the skin 133 could be presumed.

[0108] In yet another embodiment, the processor 93 determines skin 133 contact by the penetrating member 83 by detection of an acoustic signal produced by the tip 96 of the penetrating member 83 as it strikes the patient's skin 133. Detection of the acoustic signal can be measured by an acoustic detector 136 placed in contact with the patient's skin 133 adjacent a penetrating member penetration site 137, as shown in FIG. 8. Suitable acoustic detectors 136 include piezo electric transducers, microphones and the like. The acoustic detector 136 transmits an electrical signal generated by the acoustic signal to the processor 93 via electrical conductors 138. In another embodiment, contact of the penetrating member 83 with the patient's skin 133 can be determined by measurement of electrical continuity in a circuit that includes the penetrating member 83, the patient's finger 134 and an electrical contact pad 240 that is disposed on the patient's skin 133 adjacent the contact site 137 of the penetrating member 83, as shown in FIG. 8. In this embodiment, as soon as the penetrating member 83 contacts the patient's skin 133, the circuit 139 is completed and current flows through the circuit 139. Completion of the circuit 139 can then be detected by the processor 93 to confirm skin 133 contact by the penetrating member 83.

[0109] If the penetrating member 83 has not contacted the target skin 133, then the process proceeds to a timeout operation, as represented by the decision box numbered 167 in FIG. 6B. In the timeout operation, the processor 93 waits a predetermined time period. If the timeout period has not yet elapsed (a “No” outcome from the decision box 167), then the processor continues to monitor whether the penetrating member has contacted the target skin 133. The processor 93 preferably continues to monitor the position and speed of the penetrating member 83, as well as the electrical current to the appropriate coil 114-117 to maintain the desired penetrating member 83 movement.

[0110] If the timeout period elapses without the penetrating member 83 contacting the skin (a “Yes” output from the decision box 167), then it is deemed that the penetrating member 83 will not contact the skin and the process proceeds to a withdraw phase, where the penetrating member is withdrawn away from the skin 133, as discussed more fully below. The penetrating member 83 may not have contacted the target skin 133 for a variety of reasons, such as if the patient removed the skin 133 from the lancing device or if something obstructed the penetrating member 83 prior to it contacting the skin.

[0111] The processor 93 may also proceed to the withdraw phase prior to skin contact for other reasons. For example, at some point after initiation of movement of the penetrating member 83, the processor 93 may determine that the forward acceleration of the penetrating member 83 towards the patient's skin 133 should be stopped or that current to all coils 114-117 should be shut down. This can occur, for example, if it is determined that the penetrating member 83 has achieved sufficient forward velocity, but has not yet contacted the skin 133. In one embodiment, the average penetration velocity of the penetrating member 83 from the point of contact with the skin to the point of maximum penetration may be about 2.0 to about 10.0 m/s, specifically, about 3.8 to about 4.2 m/s. In another embodiment, the average penetration velocity of the penetrating member may be from about 2 to about 8 meters per second, specifically, about 2 to about 4 m/s.

[0112] The processor 93 can also proceed to the withdraw phase if it is determined that the penetrating member 83 has fully extended to the end of the power stroke of the operation cycle of lancing procedure. In other words, the process may proceed to withdraw phase when an axial center 141 of the magnetic member 102 has moved distal of an axial center 142 of the first coil 114 as shown in FIG. 5. In this situation, any continued power to any of the coils 114-117 of the driver coil pack 88 serves to decelerate the magnetic member 102 and thus the penetrating member 83. In this regard, the processor 93 considers the length of the penetrating member 83 (which can be stored in memory) the position of the penetrating member 83 relative to the magnetic member 102, as well as the distance that the penetrating member 83 has traveled.

[0113] With reference again to the decision box 165 in FIG. 6B, if the processor 93 determines that the penetrating member 83 has contacted the skin 133 (a “Yes” outcome from the decision box 165), then the processor 93 can adjust the speed of the penetrating member 83 or the power delivered to the penetrating member 83 for skin penetration to overcome any frictional forces on the penetrating member

83 in order to maintain a desired penetration velocity of the penetrating member. The flow diagram box numbered 167 represents this.

[0114] As the velocity of the penetrating member 83 is maintained after contact with the skin 133, the distal tip 96 of the penetrating member 83 will first begin to depress or tent the contacted skin 137 and the skin 133 adjacent the penetrating member 83 to form a tented portion 243 as shown in FIG. 9 and further shown in FIG. 10. As the penetrating member 83 continues to move in a distal direction or be driven in a distal direction against the patient's skin 133, the penetrating member 83 will eventually begin to penetrate the skin 133, as shown in FIG. 11. Once penetration of the skin 133 begins, the static force at the distal tip 96 of the penetrating member 83 from the skin 133 will become a dynamic cutting force, which is generally less than the static tip force. As a result in the reduction of force on the distal tip 96 of the penetrating member 83 upon initiation of cutting, the tented portion 243 of the skin 133 adjacent the distal tip 96 of the penetrating member 83 which had been depressed as shown in FIGS. 32 and 24 will spring back as shown in FIG. 11.

[0115] In the next operation, represented by the decision box numbered 171 in FIG. 6B, the processor 93 determines whether the distal end 96 of the penetrating member 83 has reached a brake depth. The brake depth is the skin penetration depth for which the processor 93 determines that deceleration of the penetrating member 83 is to be initiated in order to achieve a desired final penetration depth 144 of the penetrating member 83 as shown in FIG. 12. The brake depth may be pre-determined and programmed into the processor's memory, or the processor 93 may dynamically determine the brake depth during the actuation. The amount of penetration of the penetrating member 83 in the skin 133 of the patient may be measured during the operation cycle of the penetrating member device 80. In addition, as discussed above, the penetration depth suitable for successfully obtaining a useable sample can depend on the amount of tenting of the skin 133 during the lancing cycle. The amount of tenting of the patient's skin 133 can in turn depend on the tissue characteristics of the patient such as elasticity, hydration etc. A method for determining these characteristics is discussed below with regard to skin 133 tenting measurements during the lancing cycle and illustrated in FIGS. 37-41.

[0116] Penetration measurement can be carried out by a variety of methods that are not dependent on measurement of tenting of the patient's skin. In one embodiment, the penetration depth of the penetrating member 83 in the patient's skin 133 is measured by monitoring the amount of capacitance between the penetrating member 83 and the patient's skin 133. In this embodiment, a circuit includes the penetrating member 83, the patient's finger 134, the processor 93 and electrical conductors connecting these elements. As the penetrating member 83 penetrates the patient's skin 133, the greater the amount of penetration, the greater the surface contact area between the penetrating member 83 and the patient's skin 133. As the contact area increases, so does the capacitance between the skin 133 and the penetrating member 83. The increased capacitance can be easily measured by the processor 93 using methods known in the art and penetration depth can then be correlated to the amount

of capacitance. The same method can be used by measuring the electrical resistance between the penetrating member 83 and the patient's skin.

[0117] If the brake depth has not yet been reached, then a "No" results from the decision box 171 and the process proceeds to the timeout operation represented by the flow diagram box numbered 173. In the timeout operation, the processor 93 waits a predetermined time period. If the timeout period has not yet elapsed (a "No" outcome from the decision box 173), then the processor continues to monitor whether the brake depth has been reached. If the timeout period elapses without the penetrating member 83 achieving the brake depth (a "Yes" output from the decision box 173), then the processor 93 deems that the penetrating member 83 will not reach the brake depth and the process proceeds to the withdraw phase, which is discussed more fully below. This may occur, for example, if the penetrating member 83 is stuck at a certain depth.

[0118] With reference again to the decision box numbered 171 in FIG. 6B, if the penetrating member does reach the brake depth (a "Yes" result), then the process proceeds to the operation represented by the flow diagram box numbered 275. In this operation, the processor 93 causes a braking force to be applied to the penetrating member to thereby reduce the speed of the penetrating member 83 to achieve a desired amount of final skin penetration depth 144, as shown in FIG. 26. Note that FIGS. 32 and 33 illustrate the penetrating member making contact with the patient's skin and deforming or depressing the skin prior to any substantial penetration of the skin. The speed of the penetrating member 83 is preferably reduced to a value below a desired threshold and is ultimately reduced to zero. The processor 93 can reduce the speed of the penetrating member 83 by causing a current to be sent to a 114-117 coil that will exert an attractive braking force on the magnetic member 102 in a proximal direction away from the patient's tissue or skin 133, as indicated by the arrow 190 in FIG. 13. Such a negative force reduces the forward or distally oriented speed of the penetrating member 83. The processor 93 can determine which coil 114-117 to energize based upon the position of the magnetic member 102 with respect to the coils 114-117 of the driver coil pack 88, as indicated by the position sensor 91.

[0119] In the next operation, the process proceeds to the withdraw phase, as represented by the flow diagram box numbered 177. The withdraw phase begins with the operation represented by the flow diagram box numbered 178 in FIG. 6C. Here, the processor 93 allows the penetrating member 83 to settle at a position of maximum skin penetration 144, as shown in FIG. 12. In this regard, the processor 93 waits until any motion in the penetrating member 83 (due to vibration from impact and spring energy stored in the skin, etc.) has stopped by monitoring changes in position of the penetrating member 83. The processor 93 preferably waits until several milliseconds (ms), such as on the order of about 8 ms, have passed with no changes in position of the penetrating member 83. This is an indication that movement of the penetrating member 83 has ceased entirely. In some embodiments, the penetrating member may be allowed to settle for about 1 to about 2000 milliseconds, specifically, about 50 to about 200 milliseconds. For other embodiments, the settling time may be about 1 to about 200 milliseconds.

[0120] It is at this stage of the lancing cycle that a software method can be used to measure the amount of tenting of the patient's skin 133 and thus determine the skin 133 characteristics such as elasticity, hydration and others. Referring to FIGS. 37-41, a penetrating member 83 is illustrated in various phases of a lancing cycle with target tissue 133. FIG. 14 shows tip 96 of penetrating member 83 making initial contact with the skin 133 at the point of initial impact.

[0121] FIG. 15 illustrates an enlarged view of the penetrating member 83 making initial contact with the tissue 133 shown in FIG. 14. In FIG. 16, the penetrating member tip 96 has depressed or tented the skin 133 prior to penetration over a distance of X, as indicated by the arrow labeled X in FIG. 16. In FIG. 17, the penetrating member 83 has reached the full length of the cutting power stroke and is at maximum displacement. In this position, the penetrating member tip 96 has penetrated the tissue 133 a distance of Y, as indicated by the arrow labeled Y in FIG. 16. As can be seen from comparing FIG. 15 with FIG. 17, the penetrating member tip 96 was displaced a total distance of X plus Y from the time initial contact with the skin 133 was made to the time the penetrating member tip 96 reached its maximum extension as shown in FIG. 17. However, the penetrating member tip 96 has only penetrated the skin 133 a distance Y because of the tenting phenomenon.

[0122] At the end of the power stroke of the penetrating member 83, as discussed above with regard to box 179 of FIG. 6C, the processor 93 allows the penetrating member to settle for about 8 msec. It is during this settling time that the skin 133 rebounds or relaxes back to approximately its original configuration prior to contact by the penetrating member 83 as shown in FIG. 18. The penetrating member tip 96 is still buried in the skin to a depth of Y, as shown in FIG. 18, however the elastic recoil of the tissue has displaced the penetrating member rearward or retrograde to the point of inelastic tenting that is indicated by the arrows Z in FIG. 18. During the rearward displacement of the penetrating member 83 due to the elastic tenting of the tissue 133, the processor reads and stores the position data generated by the position sensor 91 and thus measures the amount of elastic tenting, which is the difference between X and Z.

[0123] Referring to FIG. 19, a tissue penetration sampling device 80 is shown with the controllable driver 179 of FIG. 4 coupled to a sampling module cartridge 205 and disposed within a driver housing 206. A ratchet drive mechanism 207 is secured to the driver housing 206, coupled to the sampling module cartridge 205 and configured to advance a sampling module belt 208 within the sampling module cartridge 205 so as to allow sequential use of each sampling module 209 in the sampling module belt 208. The ratchet drive mechanism 207 has a drive wheel 211 configured to engage the sampling modules 209 of the sampling module belt 208. The drive wheel 211 is coupled to an actuation lever 212 that advances the drive wheel 211 in increments of the width of a single sampling module 209. A T-slot drive coupler 213 is secured to the elongated coupler shaft 84.

[0124] A sampling module 209 is loaded and ready for use with the drive head 98 of the penetrating member 83 of the sampling module 209 loaded in the T-slot 214 of the drive coupler 213. A sampling site 215 is disposed at the distal end 216 of the sampling module 209 disposed about a penetrating member exit port 217. The distal end 216 of the sampling

module 209 is exposed in a module window 218, which is an opening in a cartridge cover 221 of the sampling module cartridge 205. This allows the distal end 216 of the sampling module 209 loaded for use to be exposed to avoid contamination of the cartridge cover 221 with blood from the lancing process.

[0125] A reader module 222 is disposed over a distal portion of the sampling module 209 that is loaded in the drive coupler 213 for use and has two contact brushes 224 that are configured to align and make electrical contact with analyte detecting member contacts 225 of the sampling module 209 as shown in FIG. 77. With electrical contact between the analyte detecting member contacts 225 and contact brushes 224, the processor 93 of the controllable driver 179 can read a signal from an analytical region 226 of the sampling module 209 after a lancing cycle is complete and a blood sample enters the analytical region 226 of the sampling module 209. The contact brushes 224 can have any suitable configuration that will allow the sampling module belt 208 to pass laterally beneath the contact brushes 224 and reliably make electrical contact with the sampling module 209 loaded in the drive coupler 213 and ready for use. A spring loaded conductive ball bearing is one example of a contact brush 224 that could be used. A resilient conductive strip shaped to press against the inside surface of the flexible polymer sheet 227 along the analyte detecting member region 228 of the sampling module 209 is another embodiment of a contact brush 224.

[0126] The sampling module cartridge 205 has a supply canister 229 and a receptacle canister 230. The unused sampling modules of the sampling module belt 208 are disposed within the supply canister 229 and the sampling modules of the sampling module belt 208 that have been used are advanced serially after use into the receptacle canister 230.

[0127] FIG. 20 illustrates a further embodiment of sampling module cartridges. FIG. 20 shows a sampling module cartridge 202 in a carousel configuration with adjacent sampling modules 204 connected rigidly and with analyte detecting members 206 from the analytical regions of the various sampling modules 204 disposed near an inner radius 208 of the carousel. The sampling modules 204 of the sampling module cartridge 202 are advanced through a drive coupler 213 but in a circular as opposed to a linear fashion.

[0128] FIG. 21 shows an exploded view in perspective of the cartridge 245, which has a proximal end portion 254 and a distal end portion 255. The penetrating member cartridge body 246 is disposed at the proximal end portion 254 of the cartridge 245 and has a plurality of penetrating member module portions 250, such as the penetrating member module portion 250. Each penetrating member module portion 250 has a penetrating member channel 251 with a penetrating member 83 slidably disposed within the penetrating member channel 251. The penetrating member channels 251 are substantially parallel to the longitudinal axis 252 of the penetrating member cartridge body 246. The penetrating members 83 shown have a drive head 98, shaft portion 201 and sharpened tip 96. The drive head 98 of the penetrating members are configured to couple to a drive coupler (not shown), such as the drive coupler 85 discussed above.

[0129] The penetrating members 83 are free to slide in the respective penetrating member channels 251 and are nomi-

nally disposed with the sharpened tip 96 withdrawn into the penetrating member channel 251 to protect the tip 96 and allow relative rotational motion between the penetrating member cartridge body 246 and the sampling cartridge body 247 as shown by arrow 256 and arrow 257 in FIG. 21. The radial center of each penetrating member channel 251 is disposed a fixed, known radial distance from the longitudinal axis 252 of the penetrating member cartridge body 246 and a longitudinal axis 258 of the cartridge 245. By disposing each penetrating member channel 251 a fixed known radial distance from the longitudinal axes 252 and 258 of the penetrating member cartridge body 246 and cartridge 245, the penetrating member channels 251 can then be readily and repeatably aligned in a functional arrangement with penetrating member channels 253 of the sampling cartridge body 247. The penetrating member cartridge body 246 rotates about a removable pivot shaft 259 which has a longitudinal axis 260 that is coaxial with the longitudinal axes 252 and 250 of the penetrating member cartridge body 246 and cartridge 245.

[0130] The sampling cartridge body 247 is disposed at the distal end portion 255 of the cartridge and has a plurality of sampling module portions 248 disposed radially about the longitudinal axis 249 of the sampling cartridge body 247. The longitudinal axis 249 of the sampling cartridge body 247 is coaxial with the longitudinal axes 252, 258 and 260 of the penetrating member cartridge body 246, cartridge 245 and pivot shaft 259. The sampling cartridge body 247 may also rotate about the pivot shaft 259. In order to achieve precise relative motion between the penetrating member cartridge body 246 and the sampling cartridge body 247, one or both of the cartridge bodies 246 and 247 may be rotatable about the pivot shaft 259, however, it is not necessary for both to be rotatable about the pivot shaft 259, that is, one of the cartridge bodies 246 and 247 may be secured, permanently or removably, to the pivot shaft 259.

[0131] The sampling cartridge body 247 includes a base 261 and a cover sheet 262 that covers a proximal surface 263 of the base forming a fluid tight seal. Each sampling module portion 248 of the sampling cartridge body 247, such as the sampling module portion 248, has a sample reservoir 264 and a penetrating member channel 253. The sample reservoir 264 has a vent 965 at an outward radial end that allows the sample reservoir 264 to readily fill with a fluid sample. The sample reservoir 264 is in fluid communication with the respective penetrating member channel 253 which extends substantially parallel to the longitudinal axis 249 of the sampling cartridge body 247. The penetrating member channel 253 is disposed at the inward radial end of the sample reservoir 264. Still further description of the device of FIG. 21 may be found in commonly assigned, copending U.S. patent application Ser. No. 10/127,395 (Attorney Docket No. 38187-2551) filed Apr. 19, 2002.

[0132] Referring to FIG. 22A, one embodiment of the present invention is a tissue penetrating system 310 with a plurality of penetrating members 312 that each have a tissue penetrating tip 314. The number of penetrating members 310 can vary, but numbers in the ranges of 10, 15, 25, 50, 75, 100, 500 or any other number, are suitable. Each penetrating member 312 can be a lancet, a traditional lancet with a molded body, a needle with a lumen, a knife like element, an elongate member without molded attachments, and the like, and may have a size in the range of 20 mm to 10 mm in

length and between 0.012-0.040 mm in diameter. It should be understood of course that penetrating members of a variety of different sizes useful for lancing such as those of conventional lancets may be used in other embodiments. As seen in FIG. 22A, the penetrating member may have an elongate portion with a bend near a proximal end of the member.

[0133] Each penetrating member 312 is coupled to a penetrating member driver 316. Suitable penetrating member drivers 316 include but are not limited to, an electric drive force member, a voice coil drive force generator, a linear voice coil device, a rotary voice coil device, and the like. Suitable drive force generators can be found in commonly assigned, copending U.S. patent application Ser. No. 10/127,395 (Attorney Docket No. 38187-2551) filed Apr. 19, 2002. In one embodiment, the penetrating member driver or drive force generator 316 may be a single actuator used to advance the penetrating member and to withdraw the member. The driver 316 may also be used to stop the penetrating member in the tissue site. Penetrating member driver 316 can be a non-spring actuator for drawing penetrating member 312 in a direction back towards penetrating member driver 316. A coupler 318 on penetrating member driver 316 is configured to engage at least a portion of an elongate portion of a penetrating member 312 in order to drive the penetrating member 312 along a path into and through target tissue 320, and then withdrawn from target tissue 320.

[0134] Referring now to FIG. 22B, the tips of the penetrating members 312 can be uncovered when they are launched into a selected target tissue 320. In one embodiment, sterility enclosures 322 are provided for covering at least the tip of each penetrating member 312. FIG. 22B shows that the enclosure may also cover the entire lancet. In one embodiment, each sterility enclosure 322 is removed from the penetrating member 312 prior to actuation, launch, of penetrating member 312 and positioned so that penetrating member 312 does not contact the associated sterility enclosure 322 during actuation. As seen in FIG. 22B, the enclosure 322 may be peel away to reveal the penetrating member 312 prior to coupling of the member 312 to the drive force generator 316. In another embodiment, each penetrating member 312 breaches its associated sterility enclosure 322 during launch.

[0135] Tissue penetrating system 310 can also include one or more penetrating member sensors 324 that are coupled to penetrating members 312. Examples of suitable penetrating member sensors 324 include but are not limited to, a capacitive incremental encoder, an incremental encoder, an optical encoder, an interference encoder, and the like. Each penetrating member sensor 324 is configured to provide information relative to a depth of penetration of a penetrating member 312 through a target tissue 320 surface, including but not limited to a skin surface, and the like. The penetrating member sensor 324 may be positioned as shown in FIG. 22B. The penetrating member sensor 324 may also be positioned in a variety of location such as but not limited to being closer to the distal end of the penetrating member, in a position as shown in FIG. 5, or in any other location useful for providing an indication of the position of a penetrating member 312 being driven by the force generator 316.

[0136] In various embodiments, the penetration depth of a penetrating member 312 through the surface of a target tissue 320 can be, 100 to 2500 microns, 500 to 750 microns, and the like. Each penetrating member sensor 324 can also provide an indication of velocity of a penetrating member 312. Referring to FIG. 22C, a damper 326 can be coupled to penetrating member driver 316. Damper 326 prevents multiple oscillations of penetrating member 312 in target tissue 320, particularly after penetrating member 312 has reached a desired depth of penetration. The damper 326 may be placed in a variety of positions such as but not limited to being coupled to the penetrating member, being coupled to the coupler 318, being coupled to a core or shaft in the drive force generator 316, or at any other position useful for slowing the motion of the penetrating member 312.

[0137] A feedback loop 328 can also be included that is coupled to penetrating member sensor 324. Each penetrating member 312 sensor can be coupled to a processor 330 that has control instructions for penetrating member driver 316. By way of illustration, and without limitation, processor 330 can include a memory for storage and retrieval of a set of penetrating member 312 profiles utilized with penetrating member driver 316. Processor 330 can also be utilized to monitor position and speed of a penetrating member 312 as it moves in first direction 332 to and through the target tissue 320.

[0138] Processor 330 can adjust an application of force to a penetrating member 312 in order to achieve a desired speed of a penetrating member 312. Additionally, processor 330 can also be used to adjust an application of force applied to a penetrating member 312 when penetrating member 312 contacts target tissue 320 so that penetrating member 312 penetrates target tissue 320 within a desired range of speed. Further, processor 330 can also monitor position and speed of a penetrating member 312 as penetrating member 312 moves in first direction 332 toward the target tissue 320. Application of a launching force to penetrating member 312 can be controlled based on position and speed of penetrating member 312. Processor 330 can control a withdraw force, from target tissue 320, to penetrating member 312 so that penetrating member 312 moves in second direction 334 away from target tissue 320.

[0139] Processor 330 can produce a signal that is indicative of a change in direction and magnitude of force exerted on penetrating member 312. Additionally, processor 330 can cause a braking force to be applied to penetrating member 312.

[0140] In one embodiment, in first direction 332 penetrating member 312 moves toward target tissue 320 at a speed that is different than a speed at which penetrating member 312 moves away from target tissue 320 in second direction 334. In one embodiment, the speed of penetrating member 312 in first direction 332 is greater than the speed of penetrating member 312 in second direction 334. The speed of penetrating member 312 in first direction 332 can be a variety of different ranges including but not limited to, 0.05 to 60 m/sec, 0.1 to 20.0 m/sec, 1.0 to 10.0 m/sec, 3.0 to 8.0 m/sec, and the like. Additionally, the dwell time of penetrating member 312 in target tissue 320, below a surface of the skin or other structure, can be in the range of, 1 microsecond to 2 seconds, 500 milliseconds to 1.5 second, 100 milliseconds to 1 second, and the like.

[0141] As seen in FIGS. 22A and 22B, tissue penetrating system 310 can include a penetrating member transport device 336 for moving each of penetrating member 312 into a position for alignment with penetrating member driver 316. Penetrating members 312 can be arranged in an array configuration by a number of different devices and structures defining support 338, including but not limited to, a belt, a flexible or non-flexible tape device, support channel, cog, a plurality of connectors, and the like. Support 338 can have a plurality of openings each receiving a penetrating member 312. Suitable supports 338 may also include but are not limited to, a bandolier, drum, disc and the like. A description of supports 338 can be found in commonly assigned, copending U.S. patent application Ser. No. 10/127,395 (Attorney Docket No. 38187-2551) filed Apr. 19, 2002; commonly assigned, copending U.S. Provisional Patent Application Ser. No. \_\_\_\_\_ (Attorney Docket No. 38187-PA Feed) filed Dec. 31, 2002; and commonly assigned, copending U.S. Provisional Patent Application Ser. No. \_\_\_\_\_ (Attorney Docket No. 38187-PA Feed) filed Dec. 31, 2002. All applications listed above are fully incorporated herein by reference for all purposes.

[0142] As illustrated in FIG. 23, tissue penetrating system 310 can include a single penetrating member driver 316 and a plurality of penetrating members 312. Penetrating member driver 316 moves each penetrating member 312 along a path out of a housing that has a penetrating member exit and then into target tissue 320, stopping in target tissue 320, and then withdrawing out of the target tissue 320. Support 338 couples the penetrating members 312 to define a linear array. Support 338 is movable and configured to move each penetrating member 312 to a launch position associated with penetrating member driver 316. Penetrating member driver 316 can be controlled to follow a predetermined velocity trajectory into and out of target tissue 320.

[0143] Tissue penetrating system 310 can include a user interface 340 configured to relay different information, including but not limited to, skin penetrating performance, a skin penetrating setting, and the like. User interface 340 can provide a user with at a variety of different outputs, including but not limited to, penetration depth of a penetrating member 312, velocity of a penetrating member 312, a desired velocity profile, a velocity of penetrating member 312 into target tissue 320, velocity of the penetrating member 312 out of target tissue 320, dwell time of penetrating member 312 in target tissue 320, a target tissue relaxation parameter, and the like. User interface 340 can include a variety of components including but not limited to, a real time clock 342, one or more alarms 344 to provide a user with a reminder of a next target penetrating event is needed, a user interface processor 346, and the like.

[0144] User interface 340 can provide a variety of different outputs to a user including but not limited to, number of penetrating members 312 available, number of penetrating members 312 used, actual depth of penetrating member 312 penetration on target tissue 320, stratum corneum thickness in the case where the target tissue 320 is the skin and an area below the skin, force delivered on target tissue 320, energy used by penetrating member driver 316 to drive penetrating member 312 into target tissue 320, dwell time of penetrating member 312, battery status of tissue penetrating system 310, status of tissue penetrating system 310, the amount of energy consumed by tissue penetrating system 310, or any compo-

nent of tissue penetrating system 310, speed profile of penetrating member 312, information relative to contact of penetrating member 312 with target tissue 320 before penetration by penetrating member 312, information relative to a change of speed of penetrating member 312 as in travels in target tissue 320, and the like.

[0145] User interface 340 can include a data interface 348 that couples tissue penetrating system 310 to support equipment 350 with an interface, the internet, and the like. The data interface 348 may also be coupled to the processor 93. Suitable support equipment 350 includes but is not limited to, a base station, home computer, central server, main processing equipment for storing analyte, such as glucose, level information, and the like.

[0146] Data interface 348 can be a variety of interfaces including but not limited to, Serial RS-232, modem interface, USB, HPNA, Ethernet, optical interface, IRDA, RF interface, Bluetooth interface, cellular telephone interface, two-way pager interface, parallel port interface standard, near field magnetic coupling, RF transceiver, telephone system, and the like.

[0147] User interface 340 be coupled to a memory 352 that stores, a target tissue parameter, target tissue 320 penetrating performance, and the like. The memory 352 may also be connected to processor 93 and store data from the user interface 340.

[0148] In one embodiment, memory 352 can store, the number of target tissue penetrating events, time and date of the last selected number of target tissue penetrating events, time interval between alarm and target tissue penetrating event, stratum corneum thickness, time of day, energy consumed by penetrating member driver 316 to drive penetrating member 312 into target tissue 320, depth of penetrating member 312 penetration, velocity of penetrating member 312, a desired velocity profile, velocity of penetrating member 312 into target tissue 320, velocity of penetrating member 312 out of target tissue 320, dwell time of penetrating member 312 in target tissue 320, a target tissue relaxation parameter, force delivered on target tissue 320 by any component of tissue penetrating device, dwell time of penetrating member 312, battery status of tissue penetrating system 310, tissue penetrating system 310 status, consumed energy by tissue penetrating system 310 or any of its components, speed profile of penetrating member 312 as it penetrates and advances through target tissue 320, a tissue target tissue relaxation parameter, information relative to contact of penetrating member 312 with target tissue 320 before penetration by penetrating member 312, information relative to a change of speed of penetrating member 312 as in travels in and through target tissue 320, information relative to consumed analyte detecting members, and information relative to consumed penetrating members 312.

[0149] In one embodiment, processor 330 is coupled to and receives any of a different type of signals from user interface 340. User interface 340 can respond to a variety of different commands, including but not limited to audio commands, and the like. User interface 340 can include a sensor for detecting audio commands. Information can be relayed to a user of tissue penetrating system 310 by way of an audio device, wireless device, and the like.

[0150] In another embodiment as seen in FIG. 23B, tissue penetrating device includes a human interface 354 with at

least one output. The human interface **354** is specific for use by humans while a user interface **340** may be for any type of user, with user defined generically. Human interface **354** can be coupled to processor **330** and penetrating member sensor **324**. Human interface **354** can be a variety of different varieties including but not limited to, LED, LED digital display, LCD display, sound generator, buzzer, vibrating device, and the like.

[0151] The output of human interface **354** can be a variety of outputs including but not limited to, a penetration event by penetrating member **312**, number of penetrating members **312** remaining, time of day, alarm, penetrating member **312** trajectory waveform profile information, force of last penetration event, last penetration event, battery status of tissue penetrating system **310**, analyte status, time to change cassette status, jamming malfunction, tissue penetrating system **310** status, and the like.

[0152] Human interface **354** is coupled to a housing **356**. Suitable housings **356** include but are not limited to, a telephone, watch, PDA, electronic device, medical device, point of care device, decentralized diagnostic device and the like. An input device **358** is coupled to housing. Suitable input devices **358** include but are not limited to, one or more pushbuttons, a touch pad independent of the display device, a touch sensitive screen on a visual display, and the like.

[0153] A data exchange device **360** can be utilized for coupling tissue penetrating system **310** to support equipment **350** including but not limited to, personal computer, modem, PDA, computer network, and the like. Human interface **354** can include a real time clock **362**, and one or more alarms **364** that enable a user to set and use for reminders for the next target tissue penetration event. Human interface **354** can be coupled to a human interface processor **366** which is distinct from processor **330**. Human interface processor **366** can include a sleep mode and can run intermittently to conserve power. Human interface processor **366** includes logic that can provide an alarm time set for a first subset of days, and a second alarm time set for a second subset of days. By way of example, and without limitation, the first subset of days can be Monday through Friday, and the second subset of days can be Saturday and Sunday.

[0154] Human interface **354** can be coupled to a memory **368** for storing a variety of information, including but not limited to, the number of target tissue penetrating events, time and date of the last selected number of target tissue penetrating events, time interval between alarm and target tissue penetrating event, stratum corneum thickness when target tissue **320** is below the skin surface and underlying tissue, time of day, energy consumed by penetrating member driver **316** to drive penetrating member **312** into target tissue **320**, depth of penetrating member **312** penetration, velocity of penetrating member **312**, a desired velocity profile, velocity of penetrating member **312** into target tissue **320**, velocity of penetrating member **312** out of target tissue **320**, dwell time of penetrating member **312** in target tissue **320**, a target tissue relaxation parameter, force delivered on target tissue **320**, dwell time of penetrating member **312**, battery status of tissue penetrating system **310** and its components, tissue penetrating system **310** status, consumed energy, speed profile of penetrating member **312** as it advances through target tissue **320**, a target tissue relaxation parameter, information relative to contact of a penetrating member **312** with

target tissue **320** before penetration by penetrating member **312**, information relative to a change of speed of penetrating member **312** as it travels in target tissue **320**, information relative to consumed sensors, information relative to consumed penetrating members **312**.

[0155] As illustrated in FIG. 24, tissue penetrating system **310** can include a penetrating member driver **316** and a plurality of cartridges **370**. Each cartridge **370** contains a penetrating member **312**. The cartridges **370** can be coupled together in an array, which can be a flexible array. A cartridge transport device **372** moves cartridges **370** into a launch position that operatively couples a penetrating member **312** to penetrating member driver **316**. A support couples cartridges **370** to define an array. A plurality of sterility enclosures **322** can be provided to at least cover tips of penetrating members **312**. Sterility enclosure **322** (shown in phantom) is removed from their associated penetrating members **312** prior to launch of the penetrating member **312**. The enclosure may be peeled away (not shown) in a manner similar to that as seen in FIG. 22B, with the enclosure **322** on one tape surface being peeled away. The enclosure **322** may be a blister sack, a sack tightly formed about each cartridge **370**, or other enclosure useful for maintaining a sterile environment about the cartridge **370** prior to actuation or launch. The enclosure **322** may contain the entire cartridge **370** or some portion of the cartridge **370** which may need to remain sterile prior to launch. During launch, enclosure or sterility barrier **322** can be breached by a device other than penetrating member **312**, or can be breached by penetrating member **312** itself. An analyte detection member, sensor, may be positioned to receive fluid from a wound created by the penetrating member **312**. The member may be on the cartridge **370** or may be on the device **80**.

[0156] Referring to FIGS. 24 and 25, one embodiment of tissue penetrating system **310** includes cartridge transport device **372** and a plurality of cartridges **370**. Each cartridge **370** is associated with a penetrating member **312**. Cartridge transport device **372** moves each cartridge **370** to a position to align the associated penetrating member **312** with penetrating member driver **316** to drive penetrating member **312** along a path into target tissue **320**. In one embodiment as seen in FIG. 25, each cartridge **370** has at least one of a distal port **374** and a proximal port **376**. A first seal **378** is positioned at distal or proximal ports. As seen in FIG. 25, the seal **378** may be placed at the distal port. First seal **378** is formed of a material that is fractured by penetrating member **312** before it is launched. A second seal **380** can be positioned at the other port. It will be appreciated that only one or both of distal and proximal ports **374** and **376** can be sealed, and that each cartridge **370** can include only one port **374** and **376**. For ease of illustration, the penetrating member **312** extending longitudinally through the lumen in the cartridge **370** is not shown. The seals **380** and **378** may be fractureable seals formed between the penetrating member and the cartridge **370**. During actuation, the seals **378** and **380** are broken. Seal **378** may be also be positioned to cover the distal port or exit port **374** without being sealed against the penetrating member (i.e. covering the port without touching the penetrating member). A third seal **381** may be positioned to cover an entrance to sample chamber **384**. The seal **381** may be configured to be broken when the penetrating member **312** is actuated. A still further seal **381A** may be placed in the lumen. The tip of a penetrating member may

be located at any position along the lumen, and may also be at or surrounded by one of the seals **378**, **381**, **381A**, or **376**.

[0157] Referring still to **FIG. 25**, a cover sheet **383** may be a flexible polymer sheet as described in commonly assigned, copending U.S. patent application Ser. No. 10/127,395 (Attorney Docket No. 38187-2551) filed Apr. 19, 2002. It should be understood of course that the sheet may be made of a variety of materials useful for coupling an analyte detecting member **390**. This allows the analyte detecting member **390** to be sterilized separately from the cartridge **370** and assembled together with the cartridge at a later time. This process may be used on certain analyte detecting members **390** that may be damaged if exposed to the sterilization process used on the cartridge **370**. Of course, some embodiments may also have the analyte detecting member **390** coupled to the cartridge **370** during sterilization. The cover sheet **383** may also form part of the seal to maintain a sterile environment about portions of the penetrating member. In other embodiments, the lumen housing penetrating member may be enclosed and not use a sheet **383** to help form a sterile environment. In still further embodiments, the sheet **383** may be sized to focus on covering sample chamber **384**.

[0158] As illustrated in **FIG. 26**, cartridge **370** has at least one port **374**. A plurality of penetrating members **312** are in cartridge **370**. Although cartridge **370** is shown in **FIG. 26** to have a linear design, the cartridge **370** may also have a curved, round, circular, triangular, or other configuration useful for positioning a penetrating member for use with a drive force generator. A seal **382** is associated with each penetrating member **312** in order to maintain each penetrating member **312** in a sterile environment in cartridge **370** prior to launch. Prior to launch, seal **382** associated with the penetrating member **312** to be launched is broken. In one embodiment, a punch (not shown) is used to push down on the seal **382** covering the port **376** of the cartridge **370**. This breaks the seal **382** and also pushes it downward, allowing the penetrating member to exit the cartridge without contacting the seal **382**. The timing of the breaking of the seal **382** may be varied so long as the penetrating member remains substantially sterile when being launched towards the tissue site **320**. In other embodiments, the port **376** may have a seal **383** that protrudes outward and is broken off by the downward motion of the punch. One or more sample chambers **384** are included in cartridge **370**. In one embodiment, each penetrating member **312** has an associated sample chamber **384**. In one embodiment, illustrated in **FIG. 27**, penetrating member **312** is extendable through an opening **386** of its associated sample chamber **384**. In some embodiments, a seal **387** may be included in the sample chamber **384**. Seals **382** and **387** may be made from a variety of materials such as but not limited to metallic foil, aluminum foil, paper, polymeric material, or laminates combining any of the above. The seals may also be made of a fractureable material. The seals may be made of a material that can easily be broken when a device applies a force thereto. The seals alone or in combination with other barriers may be used to create a sterile environment about at least the tip of the penetrating member prior to lancing or actuation.

[0159] With reference now to the embodiment of **FIG. 28**, each sample chamber **384** may have an opening **388** for transport of a body fluid into the sample chamber **384**. The size of sample chambers **384** in **FIGS. 26 through 28** can

vary. In various embodiments, sample chambers **384** are sized to receive, no more than 1.0 mL of the body fluid, no more than 0.75 mL of the body fluid, no more than 0.5 mL of the body fluid, no more than 0.25 mL of the body fluid, no more than 0.1 mL of the body fluid, and the like. It will be appreciated that sample chambers **384** can have larger or smaller sizes.

[0160] An analyte detecting member **390** may associated with each sample chamber **384**. The analyte detecting member **390** may be designed for use with a variety of different sensing techniques as described in commonly assigned, copending U.S. patent application Ser. No. 10/127,395 (Attorney Docket No. 38187-2551) filed Apr. 19, 2002. Analyte detecting member **390** can be positioned in sample chamber **384**, at an exterior of sample chamber **384**, or at other locations useful for obtaining an analyte. Analyte detecting member **390** can be in a well **392**, or merely be placed on a support.

[0161] In one embodiment, analyte detecting member **390** includes chemistries that are utilized to measure and detect glucose, and other analytes. In another embodiment, analyte detecting member **390** is utilized to detect and measure the amount of different analytes in a body fluid or sample. In various embodiments, analyte detecting member **390** determines a concentration of an analyte in a body fluid using a sample that does not exceed a volume of, 1 mL of a body fluid disposed in sample chamber **384**, 0.75 mL of a body fluid disposed in sample chamber **384**, 0.5 mL of a body fluid disposed in sample chamber **384**, 0.25 mL of a body fluid disposed in sample chamber **384**, 0.1 mL of a body fluid disposed in sample chamber **384**, and the like. For example and not by way of limitation, the sample chamber **384** may be of a size larger than the volumes above, but the analyte detecting member **390** can obtain an analyte reading using the amounts of fluid described above.

[0162] As illustrated in **FIG. 29**, tissue penetrating system **310** can include a housing member **394**, a penetrating member **312** positioned in housing member **394**, and analyte detecting member **390** coupled to a sample chamber **384**. Analyte detecting member **390** is configured to determine a concentration of an analyte in a body fluid using with a variety of different body fluid, sample, volumes. In various embodiments, the volume is less than 1 mL of body fluid disposed in sample chamber **384**, 0.75 of body fluid disposed in sample chamber **384**, 0.5 of body fluid disposed in sample chamber **384**, 0.25 of body fluid disposed in sample chamber **384**, 0.1 of body fluid disposed in sample chamber **384** and the like. Each tip of a penetrating member **312** is configured to extend through an opening of sample chamber **384**. A plurality of penetrating members **312** can be positioned in housing member **394**. Housing member **394** can be the same as cartridge **370**. Cartridge **370** can have distal and proximal ports **374** and **376**, respectively. Additionally, in this embodiment, a plurality of cartridges **370** can be provided, each associated with a penetrating member **312**.

[0163] Referring to **FIG. 30**, each penetrating member **312** has a packing density, or occupied volume, in cartridge **370**. In various embodiments, the packing density of each penetrating member **312** in cartridge **370** can be no more than, 5.0 cm<sup>3</sup>/penetrating member **312**, 4.0 cm<sup>3</sup>/penetrating member **312**, 3.0 cm<sup>3</sup>/penetrating member **312**, 2.0 cm<sup>3</sup>/penetrating member **312**, 1.0 cm<sup>3</sup>/penetrating member **312**,

0.75 cm<sup>3</sup>/penetrating member 312, 0.5 cm<sup>3</sup>/penetrating member 312, 0.25 cm<sup>3</sup>/penetrating member 312, 0.1 cm<sup>3</sup>/penetrating member 312, and the like. In other words, the volume required for each penetrating member does not exceed 5.0 cm<sup>3</sup>/penetrating member 312, 4.0 cm<sup>3</sup>/penetrating member 312, 3.0 cm<sup>3</sup>/penetrating member 312, 2.0 cm<sup>3</sup>/penetrating member 312, 1.0 cm<sup>3</sup>/penetrating member 312, 0.75 cm<sup>3</sup>/penetrating member 312, 0.5 cm<sup>3</sup>/penetrating member 312, 0.25 cm<sup>3</sup>/penetrating member 312, 0.1 cm<sup>3</sup>/penetrating member 312, and the like. So, as seen in FIG. 30, if the total package volume of the cartridge is defined as X and the cartridge includes Y number of penetrating members 312, penetrating members 312 and test area, or other unit 395, the volume for each unit does not exceed 5.0 cm<sup>3</sup>/unit, 4.0 cm<sup>3</sup>/unit, 3.0 cm<sup>3</sup>/unit, 2.0 cm<sup>3</sup>/unit, 1.0 cm<sup>3</sup>/unit, 0.75 cm<sup>3</sup>/unit, 0.5 cm<sup>3</sup>/unit, 0.25 cm<sup>3</sup>/unit, 0.1 cm<sup>3</sup>/unit, and the like.

[0164] In various embodiments, each penetrating member 312 and its associated sample chamber 384 have a combined packing density of no more than about 5.0 cm<sup>3</sup>, 4.0 cm<sup>3</sup>, 3.0 cm<sup>3</sup>, 2.0 cm<sup>3</sup>, 1.0 cm<sup>3</sup>, 0.75 cm<sup>3</sup>, 0.5 cm<sup>3</sup>, 0.25 cm<sup>3</sup>, 0.1 cm<sup>3</sup>, and the like.

[0165] With reference now to FIG. 31, tissue penetrating system 310 can have a first seal 378 formed at distal port 374 and a second seal 380 formed at proximal port 376 of cartridge 370. Prior to launching of penetrating member 312, distal seal 378 and second seal 380 maintain a distal tip of penetrating member 312 and sample chamber 384 in a sterile environment. Second seal 380 is breached, and penetrating member 312 is then launched.

[0166] As illustrated in FIG. 32, a plurality of lumens 396 can be positioned between distal port 374 and proximal port 376 of cartridge 370 for slidably receiving a penetrating member 312. Sample chamber 384 is defined by cartridge 370, has an opening 398 and is associated with penetrating member 312. First seal 378 covers distal port 374, and a second seal 380 covers proximal port 376.

[0167] In another embodiment as shown in FIG. 33, tissue penetrating system 310 includes a plurality of cartridges 370, penetrating member driver 316, and a plurality of penetrating members 312 coupled to penetrating member driver 316. Each penetrating member 312 is associated with a cartridge 370. A plurality of gas-tightly sealed enclosures 400 are coupled in an array. Each enclosure 400 fully contains at least one of cartridge 370. Enclosures 400 are configured to be advanceable on cartridge transport device 372 that individually releases cartridges 370 from sacks or enclosures 400 and loads them individually onto penetrating member driver 316. The enclosures 400 may be removed by peeling back a top portion of the tape as shown in FIG. 22B.

[0168] In another embodiment, a plurality of penetrating members 312 each have a sharpened distal tip. A penetrating member driver 316 is coupled to each penetrating member 312. A plurality of cartridges 370 are coupled in an array. Each cartridge 370 houses a penetrating member 312 and is configured to permit penetrating member driver 316 to engage each of penetrating members 312 sequentially. Each cartridge 370 has a plurality of seals positioned to provide that the sharpened distal tips remain in a sterile environment before penetrating target tissue 320. Penetrating members 312 are launched without breaking a seal using the penetrating member.

[0169] Referring now to FIG. 34, a plurality of cartridges 370 are provided, each having distal and proximal ports 374 and 376, respectively. A plurality of penetrating members 312 are each associated with a cartridge 370. Each penetrating member 312 has a sharpened distal tip and a shaft portion slidably disposed within cartridge 370. As seen in FIG. 34, the cartridges 370 may be coupled together by a connector or flexible support 403. A seal 404 is formed by a fracturable material between the penetrating member 312 and each cartridge 370. Seal 404 is positioned in at least one of distal or proximal ports 374 and 376, respectively, of cartridge 370. Cartridge transport device 372 moves each cartridge 370 to a position 405 that aligns penetrating member 312 with penetrating member driver 316 so that penetrating member 312 can be driven along a path into target tissue 320.

[0170] In another embodiment of the present invention as seen in FIG. 35, tissue penetrating system 310 includes a housing member 406, the plurality of penetrating members 312 positioned in housing member 406, and a tissue stabilizing member 408, which can also be a pressure applicator, stimulating member, stimulating vibratory member that imparts motion to a tissue surface, and the like. Tissue stabilizing member 408 can be positioned to at least partially surround an impact location of the penetrating member 312 on the target tissue 320 site. Tissue stabilizing member 408 can, enhance fluid flow from target tissue 320, stretch a target tissue 320 surface, apply a vacuum to target tissue 320, apply a force to target tissue 320 and cause target tissue 320 to press in an inward direction relative to housing member 406, apply a stimulation to target tissue 320, and the like. Tissue stabilizing member 408 can have a variety of different configurations. In one embodiment, tissue stabilizer member 408 includes a plurality of protrusions 410. In some further embodiments, a vacuum source 412 may be provided to assist the creation of a low pressure environment in the tissue stabilizing member 408 or along the fluid path to a sample chamber associated with the system 310. In some embodiments, the tissue stabilizing member 408 is mounted on the cartridge 370. In other embodiments, the member 408 may be mounted on the housing 406. The member 408 may also be pressed against the tissue site 320 and act as a pressure applicator. The member 408 may also be used against a variety of tissue including but not limited to skin or other body tissue.

[0171] Referring now to FIGS. 36 and 37, a cartridge 370 is shown with a penetrating member 312 creating a wound W in the tissue site 320. In FIG. 36, a movable capillary member 420 is extended towards the wound W as indicated by arrow 422 to gather body fluid being expressed from the wound. The fluid may be drawn to a sample chamber 384 (not shown). In FIG. 37, the wound W is created and then the entire cartridge is moved to the tissue site 320 to gather body fluid from the wound W. In some embodiments, the cartridge 370 moves towards the wound W relative to the housing 406.

[0172] Tissue penetrating systems 310 of FIGS. 22 through 37, can be utilized in a variety of different applications to detect any number of different analytes, including but not limited to glucose. The systems 310 may be used to measure potassium, other ions, or analytes associated with

the process of glucose monitoring. The analyte detecting member 390 may further be adapted to measure other analytes found in body fluid.

[0173] In a still further embodiment, penetrating member 312 may be moved and positioned to be in engagement with penetrating member driver 316. Penetrating member 312 is in a sterile environment, and prior to launch, the sterilizing covering, which can be a seal is removed. Tissue stabilizing member can apply a stimulation to a surface of the target tissue 320 prior to, and during penetration by penetration member. Penetrating member 312 is engaged with penetrating driving member and controllably pierces a target tissue 320 site. Penetrating member sensor 324 is utilized to control penetration depth and velocity of penetrating member 312. Penetrating member 312 is stopped at a desired depth below a surface of target tissue 320 in order to reduce or eliminate without multiple oscillations against the surface of target tissue 320. A wound is created, causing blood to flow into sample chamber 384. In various embodiments, no more than 1 mL of a body fluid is collected in sample chamber 384.

[0174] A number of different preferences, options, embodiment, and features have been given above, and following any one of these may results in an embodiment of this invention that is more presently preferred than a embodiment in which that particular preference is not followed. These preferences, options, embodiment, and features may be generally independent, and additive; and following more than one of these preferences may result in a more presently preferred embodiment than one in which fewer of the preferences are followed.

[0175] While the invention has been described and illustrated with reference to certain particular embodiments thereof, those skilled in the art will appreciate that various adaptations, changes, modifications, substitutions, deletions, or additions of procedures and protocols may be made without departing from the spirit and scope of the invention. Any of the embodiments of the invention may be modified to include any of the features described above or feature incorporated by reference herein. For example, the cartridge of FIG. 26 may be adapted to include a distal portion with a tissue stabilizing member. The cartridge of FIG. 26 may be adapted for use with a vacuum device. The cartridge may include indexing features such as notches on the distal portion or outer radial periphery for those cartridges with a radial configuration. The notches will facilitate positioning, among other things, and may be used for movement. Other cartridges or tapes herein may be modified with notches or tractor holes to facilitate movement. User interfaces, human interfaces, and other interfaces may be added to any of the embodiments of the present invention.

[0176] With any of the above embodiments, the location of the penetrating member drive device may be varied, relative to the penetrating members or the cartridge. With any of the above embodiments, the penetrating member tips may be uncovered during actuation (i.e. penetrating members do not pierce the penetrating member enclosure or protective foil during launch). With any of the above embodiments, the penetrating members may be a bare penetrating member during launch. With any of the above embodiments, the penetrating members may be bare penetrating members prior to launch as this may allow for

significantly tighter densities of penetrating members. In some embodiments, the penetrating members may be bent, curved, textured, shaped, or otherwise treated at a proximal end or area to facilitate handling by an actuator. The penetrating member may be configured to have a notch or groove to facilitate coupling to a gripper or coupler. The notch or groove may be formed along an elongate portion of the penetrating member. The coupler may be designed to create a frictional only type grip on the penetrating member.

[0177] With any of the above embodiments, any open cavity housing the penetrating may be on the bottom or the top of the cartridge, with the gripper on the other side. In some embodiments, sensors may be printed on the top, bottom, or side of the cavities. The front end of the cartridge maybe in contact with a user during lancing. The same driver may be used for advancing and retraction of the penetrating member. The penetrating member may have a diameters and length suitable for obtaining the blood volumes described herein. The penetrating member driver may also be in substantially the same plane as the cartridge. The driver may use a through hole or other opening to engage a proximal end of a penetrating member to actuate the penetrating member along a path into and out of the tissue.

[0178] Any of the features described in this application or any reference disclosed herein may be adapted for use with any embodiment of the present invention. For example, the devices of the present invention may also be combined for use with injection penetrating members or needles as described in commonly assigned, copending U.S. patent application Ser. No. 10/127,395 (Attorney Docket No. 38187-2551) filed Apr. 19, 2002. A sensor to detect the presence of foil may also be included in the lancing apparatus. For example, if a cavity has been used before, the foil or sterility barrier will be punched. The sensor can detect if the cavity is fresh or not based on the status of the barrier. It should be understood that in optional embodiments, the sterility barrier may be designed to pierce a sterility barrier of thickness that does not dull a tip of the penetrating member. The lancing apparatus may also use improved drive mechanisms. For example, a solenoid force generator may be improved to try to increase the amount of force the solenoid can generate for a given current. A solenoid for use with the present invention may have five coils and in the present embodiment the slug is roughly the size of two coils. One change is to increase the thickness of the outer metal shell or windings surround the coils. By increasing the thickness, the flux will also be increased. The slug may be split; two smaller slugs may also be used and offset by  $\frac{1}{2}$  of a coil pitch. This allows more slugs to be approaching a coil where it could be accelerated. This creates more events where a slug is approaching a coil, creating a more efficient system.

[0179] In another optional alternative embodiment, a gripper in the inner end of the protective cavity may hold the penetrating member during shipment and after use, eliminating the feature of using the foil, protective end, or other part to retain the used penetrating member. Some other advantages of the disclosed embodiments and features of additional embodiments include: same mechanism for transferring the used penetrating members to a storage area; a high number of penetrating members such as 25, 50, 75, 100, 500, or more penetrating members may be put on a disk or cartridge; molded body about a penetrating member

becomes unnecessary; manufacturing of multiple penetrating member devices is simplified through the use of cartridges; handling is possible of bare rods metal wires, without any additional structural features, to actuate them into tissue; maintaining extreme (better than 50 micron-lateral- and better than 20 micron vertical) precision in guiding; and storage system for new and used penetrating members, with individual cavities/slots is provided. The housing of the lancing device may also be sized to be ergonomically pleasing. In one embodiment, the device has a width of about 56 mm, a length of about 105 mm and a thickness of about 15 mm. Additionally, some embodiments of the present invention may be used with non-electrical force generators or drive mechanism. For example, the punch device and methods for releasing the penetrating members from sterile enclosures could be adapted for use with spring based launchers. The gripper using a frictional coupling may also be adapted for use with other drive technologies.

**[0180]** Still further optional features may be included with the present invention. For example, with any of the above embodiments, the location of the penetrating member drive device may be varied, relative to the penetrating members or the cartridge. With any of the above embodiments, the penetrating member tips may be uncovered during actuation (i.e. penetrating members do not pierce the penetrating member enclosure or protective foil during launch). The penetrating members may be a bare penetrating member during launch. The same driver may be used for advancing and retraction of the penetrating member. Different analyte detecting members detecting different ranges of glucose concentration, different analytes, or the like may be combined for use with each penetrating member. Non-potentiometric measurement techniques may also be used for analyte detection. For example, direct electron transfer of glucose oxidase molecules adsorbed onto carbon nanotube powder microelectrode may be used to measure glucose levels. In all methods, nanoscopic wire growth can be carried out via chemical vapor deposition (CVD). In all of the embodiments of the invention, preferred nanoscopic wires may be nanotubes. Any method useful for depositing a glucose oxidase or other analyte detection material on a nanowire or nanotube may be used with the present invention. Expected variations or differences in the results are contemplated in accordance with the objects and practices of the present invention. It is intended, therefore, that the invention be defined by the scope of the claims which follow and that such claims be interpreted as broadly as is reasonable.

What is claimed is:

1. A tissue penetration device, comprising:

a penetrating member driver;

a cartridge;

a plurality of penetrating members integrated with the cartridge, each of penetrating member coupled to the penetrating member driver when advanced along a path into a tissue target; and

a penetrating member sensor coupled to the plurality of penetrating members, the penetrating member sensor configured to provide information relative to a depth of penetration of a penetrating member through a skin surface.

2. The system of claim 1, wherein the depth of penetration is 100 to 2500 microns.

3. The system of claim 1, wherein the depth of penetration is 500 to 750 microns.

4. The system of claim 1, wherein the penetrating member sensor is further configured to provide an indication of velocity of a penetrating member.

5. The system of claim 1, further comprising:

a second penetrating member sensor configured to provide an indication of velocity of a penetrating member.

6. The system of claim 1, further comprising:

a feedback loop coupled to the penetrating member sensor.

7. The system of claim 1, wherein the penetrating member driver is an electric drive force member.

8. The system of claim 1, wherein the penetrating member driver is a voice coil drive force generator.

9. The system of claim 1, wherein the penetrating member sensor is coupled to a processor with control instructions for the penetrating member driver.

10. The system of claim 9, wherein the processor includes a memory for storage and retrieval of a set of penetrating member profiles utilized with the penetrating member driver.

11. The system of claim 9, wherein the processor is utilized to monitor position and speed of a penetrating member as the penetrating member moves in a first direction.

12. The system of claim 9, wherein the processor is utilized to adjust an application of force to a penetrating member to achieve a desired speed of the penetrating member.

13. The system of claim 9, wherein the processor is utilized to adjust an application of force to a penetrating member when the penetrating member contacts a target tissue so that the penetrating member penetrates the target tissue within a desired range of speed.

14. The system of claim 9, wherein the processor is utilized to monitor position and speed of a penetrating member as the penetrating member moves in the first direction toward a target tissue, wherein the application of a launching force to the penetrating member is controlled based on position and speed of the penetrating member.

15. The system of claim 14, wherein the processor is utilized to control a withdraw force to the penetrating member so that the penetrating member moves in a second direction away from the target tissue.

16. The system of claim 15, wherein in the first direction the penetrating member moves toward the target tissue at a speed that is different than a speed at which the penetrating member moves away from the target tissue.

17. The system of claim 15, wherein in the first direction the penetrating member moves toward the target tissue at a speed that is greater than a speed at which the penetrating member moves away from the target tissue.

18. The system of claim 14, wherein a speed of a penetrating member in the first direction is the range of 0.05 to 60 m/sec.

19. The system of claim 14, wherein a speed of a penetrating member in the first direction is the range of 0.1 to 20.0 m/sec.

20. The system of claim 14, wherein a speed of a penetrating member in the first direction is the range of 1.0 to 10.0 m/sec.

21. The system of claim 14, wherein a speed of a penetrating member in the first direction is the range of 3.0 to 8.0 m/sec.

22. The system of claim 14, wherein a dwell time of the penetrating member in the target tissue below a skin surface is in the range of 1 microsecond to 2 seconds.

23. The system of claim 1, wherein a dwell time of the penetrating member in the target tissue below a skin surface is in the range of 500 milliseconds to 1.5 second.

24. The system of claim 1, wherein a dwell time of the penetrating member in the target tissue below a skin surface is in the range of 100 milliseconds to 1 second.

25. The system of claim 1, further comprising:

a plurality of cartridges integrated in a cassette.

26. The system of claim 25, wherein each cartridge has an exit port, and upon launch each penetrating member exists from the exit port.

27. The system of claim 1, wherein the penetrating member sensor includes a capacitive incremental encoder.

28. The system of claim 1, wherein the penetrating member sensor includes an incremental encoder.

29. The system of claim 1, wherein the penetrating member sensor includes an optical encoder.

30. The system of claim 1, wherein the penetrating member sensor includes an interference encoder.

31. The system of claim 1, further comprising:

an analyte detecting member.

32. The system of claim 1, further comprising:

a plurality of analyte detecting members each coupled to a penetrating member.

33. The system of claim 1, further comprising:

a sample chamber with an opening for transport of a body fluid into the sample chamber, the sample chamber being sized to receive no more than 1.0  $\mu\text{L}$  of the body fluid.

34. The system of claim 1, further comprising:

a sample chamber with an opening for transport of a body fluid into the sample chamber, the sample chamber being sized to receive no more than 0.75  $\mu\text{L}$  of the body fluid.

35. The system of claim 1, further comprising:

a sample chamber with an opening for transport of a body fluid into the sample chamber, the sample chamber being sized to receive no more than 0.5  $\mu\text{L}$  of the body fluid.

36. The system of claim 1, further comprising:

a sample chamber with an opening for transport of a body fluid into the sample chamber, the sample chamber being sized to receive no more than 0.25  $\mu\text{L}$  of the body fluid.

37. The system of claim 1, further comprising:

a sample chamber with an opening for transport of a body fluid into the sample chamber, the sample chamber being sized to receive no more than 0.1  $\mu\text{L}$  of the body fluid.

38. The system of claim 1, further comprising:

an analyte detecting member coupled to a sample chamber, the analyte detecting member being configured to determine a concentration of an analyte in a body fluid using a sample that does not exceed a volume of 1  $\mu\text{L}$  of a body fluid disposed in the sample chamber.

39. The system of claim 1, further comprising:

an analyte detecting member coupled to a sample chamber, the analyte detecting member being configured to determine a concentration of an analyte in a body fluid using a sample that does not exceed a volume of 0.75  $\mu\text{L}$  of a body fluid disposed in the sample chamber.

40. The system of claim 1, further comprising:

an analyte detecting member coupled to a sample chamber, the analyte detecting member being configured to determine a concentration of an analyte in a body fluid using a sample that does not exceed a volume of 0.5  $\mu\text{L}$  of a body fluid disposed in the sample chamber.

41. The system of claim 1, further comprising:

an analyte detecting member coupled to a sample chamber, the analyte detecting member being configured to determine a concentration of an analyte in a body fluid using a sample that does not exceed a volume of 0.25  $\mu\text{L}$  of a body fluid disposed in the sample chamber.

42. The system of claim 1, further comprising:

an analyte detecting member coupled to a sample chamber, the analyte detecting member being configured to determine a concentration of an analyte in a body fluid using a sample that does not exceed a volume of 0.1  $\mu\text{L}$  of a body fluid disposed in the sample chamber.

43. The system of claim 1, wherein each of a penetrating member of the plurality of penetrating members has a packing density of no more than 1.0  $\text{cm}^3/\text{penetrating member}$ .

44. The system of claim 1, wherein each of a penetrating member of the plurality of penetrating members has a packing density of no more than 0.75  $\text{cm}^3/\text{penetrating member}$ .

45. The system of claim 1, wherein the each of a penetrating member of the plurality of penetrating members has a packing density of no more than 0.5  $\text{cm}^3/\text{penetrating member}$ .

46. The system of claim 1, wherein each of a penetrating member of the plurality of penetrating members has a packing density of no more than 0.25  $\text{cm}^3/\text{penetrating member}$ .

47. The system of claim 1, wherein each of a penetrating member of the plurality of penetrating members has a packing density of no more than 0.1  $\text{cm}^3/\text{penetrating member}$ .

48. The system of claim 33, wherein each of a penetrating member and an associated sample chamber have a combined packing density of no more than 1.0  $\text{cm}^3$ .

49. The system of claim 33, wherein each of a penetrating member and an associated sample chamber have a combined packing density of no more than 0.75  $\text{cm}^3$ .

50. The system of claim 33, wherein each of a penetrating member and an associated sample chamber have a combined packing density of no more than 0.5  $\text{cm}^3$ .

51. The system of claim 33, wherein each of a penetrating member and an associated sample chamber have a combined packing density of no more than 0.25  $\text{cm}^3$ .

**52.** The system of claim 33, wherein each of a penetrating member and an associated sample chamber have a combined packing density of no more than  $0.1 \text{ cm}^3$

**53.** The system of claim 1, further comprising:

a tissue stabilizer device coupled to the housing.

**54.** The system of claim 53, wherein the tissue stabilizer device is configured to enhance fluid flow from a target tissue.

**55.** The system of claim 53, wherein the tissue stabilizer device creates a stretching of a skin surface.

**56.** The system of claim 53, wherein the tissue stabilizer device includes a plurality of protrusions.

**57.** The system of claim 53, wherein the tissue stabilizer device applies a vacuum to a target tissue.

**58.** The system of claim 53, wherein the tissue stabilizer device is configured to apply a force to a target tissue and cause the target tissue to press in an inward direction relative to the housing member.

**59.** The system of claim 53, wherein the tissue stabilizing member applies a stimulation to a target tissue.

**60.** The system of claim 1, further comprising:

a seal formed by a fracturable material between the penetrating member and the cartridge, the seal being positioned at least one of a distal port or a proximal port of the cartridge.

**61.** The system of claim 53, further comprising

a second fracturable seal located at least one of the distal port or proximal port of cartridge.

**62.** The system of claim 1, wherein each penetrating member each penetrating members is an elongate member without molded attachments.

**63.** The system of claim 1, further comprising:

a penetrating member transport device for moving each of a penetrating member into a position aligned with the penetrating member driver.

**64.** The system of claim 1, further comprising,

a belt for holding the penetrating members in an array configuration.

**65.** The system of claim 1, further comprising:

a tape device configured to hold the penetrating members in an array configuration.

**66.** The system of claim 1, further comprising:

a support channel configured to hold the penetrating members in an array configuration.

**67.** The system of claim 1, further comprising:

a cog configured to hold the penetrating members in an array configuration.

**68.** The system of claim 1, further comprising:

a plurality of connectors between penetrating members for holding the penetrating members in an array configuration.

**69.** The system of claim 1, further comprising:

a support structure for receiving the penetrating members.

**70.** The system of claim 69, wherein the support structure is a bandolier.

**71.** The system of claim 69, wherein the support structure is a drum.

**72.** The system of claim 69, wherein the support structure is a disc.

**73.** A tissue penetrating system, comprising:

a plurality of penetrating members;

a penetrating member driver coupled to the plurality of penetrating members;

a cartridge transport device; and

a plurality of cartridges each associated with a penetrating member, the cartridge transport device being configured to move each cartridge to a position aligning a penetrating member with the penetrating member driver to drive the penetrating member along a path into a target tissue site.

**74.** The system of claim 73, further comprising:

a penetrating member sensor coupled to the plurality of penetrating members, the penetrating member sensor configured to provide information relative to a depth of penetration of a penetrating member through a skin surface.

**75.** The system of claim 73, wherein the depth of penetration is 100 to 2500 microns.

**76.** The system of claim 73, wherein the depth of penetration is 500 to 750 microns.

**77.** The system of claim 73, wherein the penetrating member sensor is further configured to provide an indication of velocity of a penetrating member.

**78.** The system of claim 73, further comprising:

a second penetrating member sensor configured to provide an indication of velocity of a penetrating member.

**79.** The system of claim 73, further comprising:

a feedback loop coupled to the penetrating member sensor.

**80.** The system of claim 73, wherein the penetrating member driver is an electric drive force member.

**81.** The system of claim 73, wherein the penetrating member driver is a voice coil drive force generator.

**82.** The system of claim 73, wherein the penetrating member sensor is coupled to a processor with control instructions for the penetrating member driver.

**83.** The system of claim 82, wherein the processor includes a memory for storage and retrieval of a set of penetrating member profiles utilized with the penetrating member driver.

**84.** The system of claim 82, wherein the processor is utilized to monitor position and speed of a penetrating member as the penetrating member moves in a first direction.

**85.** The system of claim 82, wherein the processor is utilized to adjust an application of force to a penetrating member to achieve a desired speed of the penetrating member.

**86.** The system of claim 82, wherein the processor is utilized to adjust an application of force to a penetrating member when the penetrating member contacts a target tissue so that the penetrating member penetrates the target tissue within a desired range of speed.

**87.** The system of claim 82, wherein the processor is utilized to monitor position and speed of a penetrating member as the penetrating member moves in the first direction toward a target tissue, wherein the application of a launching force to the penetrating member is controlled based on position and speed of the penetrating member.

**88.** The system of claim 87, wherein the processor is utilized to control a withdraw force to the penetrating member so that the penetrating member moves in a second direction away from the target tissue.

**89.** The system of claim 88, wherein in the first direction the penetrating member moves toward the target tissue at a speed that is different than a speed at which the penetrating member moves away from the target tissue.

**90.** The system of claim 88, wherein in the first direction the penetrating member moves toward the target tissue at a speed that is greater than a speed at which the penetrating member moves away from the target tissue.

**91.** The system of claim 87, wherein a speed of a penetrating member in the first direction is the range of 0.05 to 60 m/sec.

**92.** The system of claim 87, wherein a speed of a penetrating member in the first direction is the range of 0.1 to 20.0 m/sec.

**93.** The system of claim 87, wherein a speed of a penetrating member in the first direction is the range of 1.0 to 10.0 m/sec.

**94.** The system of claim 87, wherein a speed of a penetrating member in the first direction is the range of 3.0 to 8.0 m/sec.

**95.** The system of claim 87, wherein a dwell time of the penetrating member in the target tissue below a skin surface is in the range of 1 microsecond to 2 seconds.

**96.** The system of claim 73, wherein a dwell time of the penetrating member in the target tissue below a skin surface is in the range of 500 milliseconds to 1.5 second.

**97.** The system of claim 73, wherein a dwell time of the penetrating member in the target tissue below a skin surface is in the range of 100 milliseconds to 1 second.

**98.** The system of claim 73, further comprising:

a plurality of cartridges integrated in a cassette.

**99.** The system of claim 98, wherein each cartridge has an exit port, and upon launch each penetrating member exists from the exit port.

**100.** The system of claim 73, wherein the penetrating member sensor includes a capacitive incremental encoder.

**101.** The system of claim 73, wherein the penetrating member sensor includes an incremental encoder.

**102.** The system of claim 73, wherein the penetrating member sensor includes an optical encoder.

**103.** The system of claim 73, wherein the penetrating member sensor includes an interference encoder.

**104.** The system of claim 73, further comprising:

an analyte detecting member.

**105.** The system of claim 73, further comprising:

a plurality of analyte detecting members each coupled to a penetrating member.

**106.** The system of claim 73, further comprising:

a sample chamber with an opening for transport of a body fluid into the sample chamber, the sample chamber being sized to receive no more than 1.0  $\mu\text{L}$  of the body fluid.

**107.** The system of claim 73, further comprising:

a sample chamber with an opening for transport of a body fluid into the sample chamber, the sample chamber being sized to receive no more than 0.75  $\mu\text{L}$  of the body fluid.

**108.** The system of claim 73, further comprising:

a sample chamber with an opening for transport of a body fluid into the sample chamber, the sample chamber being sized to receive no more than 0.5  $\mu\text{L}$  of the body fluid.

**109.** The system of claim 73, further comprising:

a sample chamber with an opening for transport of a body fluid into the sample chamber, the sample chamber being sized to receive no more than 0.25  $\mu\text{L}$  of the body fluid.

**110.** The system of claim 73, further comprising:

a sample chamber with an opening for transport of a body fluid into the sample chamber, the sample chamber being sized to receive no more than 0.1  $\mu\text{L}$  of the body fluid.

**111.** The system of claim 73, further comprising:

an analyte detecting member coupled to a sample chamber, the analyte detecting member being configured to determine a concentration of an analyte in a body fluid using a sample of less than 1  $\mu\text{L}$  of a body fluid disposed in the sample chamber.

**112.** The system of claim 111, wherein the analyte detecting member is configured to determine a concentration of an analyte in a body fluid using a sample of less than 0.5  $\mu\text{L}$  of a body fluid disposed in the sample chamber.

**113.** The system of claim 73, further comprising:

an analyte detecting member coupled to a sample chamber, the analyte detecting member being configured to determine a concentration of an analyte in a body fluid using a sample that does not exceed a volume of 0.5  $\mu\text{L}$  of a body fluid disposed in the sample chamber.

**114.** The system of claim 73, further comprising:

an analyte detecting member coupled to a sample chamber, the analyte detecting member being configured to determine a concentration of an analyte in a body fluid using a sample that does not exceed a volume of 0.25  $\mu\text{L}$  of a body fluid disposed in the sample chamber.

**115.** The system of claim 73, further comprising:

an analyte detecting member coupled to a sample chamber, the analyte detecting member being configured to determine a concentration of an analyte in a body fluid using a sample that does not exceed a volume of 0.1  $\mu\text{L}$  of a body fluid disposed in the sample chamber.

**116.** The system of claim 73, wherein each of a penetrating of the plurality of penetrating members has a packing density of no more than 1.0  $\text{cm}^3/\text{penetrating member}$ .

**117.** The system of claim 73, wherein each of a penetrating member of the plurality of penetrating members has a packing density of no more than 0.75  $\text{cm}^3/\text{penetrating member}$ .

**118.** The system of claim 73, wherein the each of a penetrating member of the plurality of penetrating members has a packing density of no more than 0.5  $\text{cm}^3/\text{penetrating member}$ .

**119.** The system of claim 73, wherein each of a penetrating member of the plurality of penetrating members has a packing density of no more than 0.25  $\text{cm}^3/\text{penetrating member}$ .

**120.** The system of claim 73, wherein each of a penetrating member of the plurality of penetrating members has a packing density of no more than  $0.1 \text{ cm}^3/\text{penetrating member}$ .

**121.** The system of claim 106, wherein each of a penetrating member and an associated sample chamber have a combined packing density of no more than  $1.0 \text{ cm}^3$ .

**122.** The system of claim 106, wherein each of a penetrating member and an associated sample chamber have a combined packing density of no more than  $0.75 \text{ cm}^3$ .

**123.** The system of claim 106, wherein each of a penetrating member and an associated sample chamber have a combined packing density of no more than  $0.5 \text{ cm}^3$ .

**124.** The system of claim 106, wherein each of a penetrating member and an associated sample chamber have a combined packing density of no more than  $0.25 \text{ cm}^3$ .

**125.** The system of claim 106, wherein each of a penetrating member and an associated sample chamber have a combined packing density of no more than  $0.1 \text{ cm}^3$ .

**126.** The system of claim 73, wherein the plurality of penetrating members have a packing density of no more than  $0.5 \text{ cm}^3/\text{penetrating member}$ .

**127.** The system of claim 73, wherein the plurality of penetrating members have a packing density of no more than  $0.1 \text{ cm}^3/\text{penetrating member}$ .

**128.** The system of claim 111, wherein the plurality of penetrating members and analyte detecting members have a packing density of no more than  $0.5 \text{ cm}^3/\text{penetrating member and analyte detecting member combination}$ .

**129.** The system of claim 111, wherein the plurality of penetrating members and analyte detecting members have a packing density of no more than  $0.1 \text{ cm}^3/\text{penetrating member and analyte detecting member combination}$ .

**130.** The system of claim 73, further comprising:

a tissue stabilizer device coupled to the housing.

**131.** The system of claim 130, wherein the tissue stabilizer device is configured to enhance fluid flow from a target tissue.

**132.** The system of claim 130, wherein the tissue stabilizer device creates a stretching of a skin surface.

**133.** The system of claim 130, wherein the tissue stabilizer device includes a plurality of protrusions.

**134.** The system of claim 130, wherein the tissue stabilizer device applies a vacuum to a target tissue.

**135.** The system of claim 130, wherein the tissue stabilizer device is configured to apply a force to a target tissue and cause the target tissue to press in an inward direction relative to the housing member.

**136.** The system of claim 130, wherein the tissue stabilizing member applies a stimulation to a target tissue.

**137.** The system of claim 73, further comprising:

a seal formed by a fracturable material between the penetrating member and a cartridge, the seal being positioned at least one of a distal port or a proximal port of the cartridge.

**138.** The system of claim 130, further comprising

a second fracturable seal located at least one of the distal port or proximal port of a cartridge.

**139.** The system of claim 73, wherein each penetrating member each penetrating members is an elongate member without molded attachments.

**140.** The system of claim 73, further comprising,

a belt for holding the penetrating members in an array configuration.

**141.** The system of claim 73, further comprising:

a tape device configured to hold the penetrating members in an array configuration.

**142.** The system of claim 73, further comprising:

a support channel configured to hold the penetrating members in an array configuration.

**143.** The system of claim 73, further comprising:

a cog configured to hold the penetrating members in an array configuration.

**144.** The system of claim 73, further comprising:

a plurality of connectors between penetrating members for holding the penetrating members in an array configuration.

**145.** The system of claim 73, further comprising:

a support structure for receiving the penetrating members.

**146.** The system of claim 145, wherein the support structure is a bandolier

**147.** The system of claim 146, wherein the support structure is a drum.

**148.** The system of claim 146, wherein the support structure is a disc.

**149.** A tissue penetrating device, comprising:

a penetrating member;

a penetrating member driver coupled to the penetrating member;

a penetrating member sensor coupled to the penetrating member, the penetrating member sensor configured to provide information relative to a depth of penetration of a penetrating member through a skin surface; and

a processor coupled to the penetrating member sensor, the processor producing a signal indicative of a change in direction and magnitude of force exerted on the penetrating member, the processor further configured to cause application of a braking force to the penetrating member.

**150.** The system of claim 149, wherein the braking force is utilized to assist in achieving a desired amount of skin penetration depth by the penetrating member.

**151.** The system of claim 149, wherein the braking force reduces multiple oscillations of the penetrating member a target tissue.

**152.** The system of claim 149, further comprising: a user interface configured to relay at least one of, skin penetrating performance or a skin penetrating setting.

**153.** The system of claim 149, further comprising:

a user interface configured to relay at least one of, skin penetrating performance or a skin penetrating setting.

**154.** The system of claim 149, further comprising:

a human interface coupled to the penetrating member driver and providing at least one output.

**155.** A skin penetrating device, comprising:

a penetrating member driver;

a penetrating member coupled to the penetrating member driver; and

a damper coupled to the penetrating member driver for preventing multiple oscillations of the penetrating member in the tissue target once the penetrating member has reached a desired depth.

**156.** The system of claim 155, further comprising:

a penetrating member sensor coupled to the penetrating member, the penetrating member sensor configured to provide information relative to a depth of penetration of a penetrating member through a skin surface.

**157.** The system of claim 155, further comprising:

a user interface configured to relay at least one of, skin penetrating performance or a skin penetrating setting.

**158.** The system of claim 155, further comprising:

a human interface coupled to the penetrating member driver and providing at least one output.

**159.** A method of penetrating a target tissue, comprising:

advancing a penetrating member through the target tissue;

stopping the penetrating member at a desired depth below a skin surface without multiple oscillations against the skin surface; and

withdrawing the penetrating member from the target tissue.

**160.** The method of claim 159, further comprising:

monitoring position and speed of the penetrating member as the penetrating member moves in the first direction toward the target tissue.

**161.** The method of claim 159, further comprising:

adjusting an application of force to the penetrating member to achieve a desired speed of the penetrating member.

**162.** The method of claim 159, further comprising:

adjusting an application of force to the penetrating member when the penetrating member contacts the skin surface so that the penetrating member penetrates the skin surface within a desired range of speed.

**163.** The method of claim 159, further comprising:

monitoring position and speed of the penetrating member as the penetrating member moves in a first direction toward the target tissue, wherein the application of a launching force to the penetrating member is controlled based on position and speed of the penetrating member.

**164.** The method of claim 163, further comprising:

controlling a withdraw force to the penetrating member so that the penetrating member moves in a second direction away from the target tissue.

**165.** A method of penetrating a target tissue, comprising:

providing a tissue penetrating system including a penetrating member driver, a plurality of cartridges, a plurality of penetrating members each associated with a cartridge, a plurality of sample chambers each associated with a penetrating member, and a penetrating member sensor;

advancing a penetrating member from a cartridge into the target tissue;

withdrawing the penetrating member from the target tissue; and

receiving an analyte sample in a sample chamber.

**166.** The method of claim 165, further comprising:

monitoring position and speed of the penetrating member as the penetrating member moves in the first direction toward the target tissue.

**167.** The method of claim 165, further comprising:

adjusting an application of force to the penetrating member to achieve a desired speed of the penetrating member.

**168.** The method of claim 165, further comprising:

adjusting an application of force to the penetrating member when the penetrating member contacts the skin surface so that the penetrating member penetrates the skin surface within a desired range of speed.

**169.** The method of claim 165, further comprising:

monitoring position and speed of the penetrating member as the penetrating member moves in a first direction toward the target tissue, wherein the application of a launching force to the penetrating member is controlled based on position and speed of the penetrating member.

**170.** The method of claim 168, further comprising:

controlling a withdraw force to the penetrating member so that the penetrating member moves in a second direction away from the target tissue.

\* \* \* \* \*