



US008695866B2

(12) **United States Patent**
Leimbach et al.

(10) **Patent No.:** **US 8,695,866 B2**
(45) **Date of Patent:** **Apr. 15, 2014**

(54) **SURGICAL INSTRUMENT HAVING A
POWER CONTROL CIRCUIT**

(75) Inventors: **Richard L. Leimbach**, Cincinnati, OH
(US); **Richard F. Schwemberger**,
Cincinnati, OH (US); **Brett E.
Swensgard**, West Chester, OH (US)

(73) Assignee: **Ethicon Endo-Surgery, Inc.**, Cincinnati,
OH (US)

(*) Notice: Subject to any disclaimer, the term of this
patent is extended or adjusted under 35
U.S.C. 154(b) by 545 days.

5,480,089 A	1/1996	Blewett
5,482,197 A	1/1996	Green et al.
5,485,952 A	1/1996	Fontayne
5,487,499 A	1/1996	Sorrentino et al.
5,497,933 A	3/1996	DeFonzo et al.
5,505,363 A	4/1996	Green et al.
5,529,235 A	6/1996	Boiarski et al.
5,535,934 A	7/1996	Boiarski et al.
5,540,375 A	7/1996	Bolanos et al.
5,542,594 A	8/1996	McKean et al.
5,551,622 A	9/1996	Yoon
5,562,241 A	10/1996	Knodel et al.
5,564,615 A	10/1996	Bishop et al.

(Continued)

FOREIGN PATENT DOCUMENTS

(21) Appl. No.: **12/896,381**

CA	2458946 A1	3/2003
CA	2512960 A1	1/2006

(22) Filed: **Oct. 1, 2010**

(Continued)

(65) **Prior Publication Data**

US 2012/0080477 A1 Apr. 5, 2012

(51) **Int. Cl.**
A61B 17/068 (2006.01)

(52) **U.S. Cl.**
USPC **227/175.2; 227/178.1; 227/175.1;**
227/2

(58) **Field of Classification Search**
USPC 227/175.1, 178.1, 2, 175.2
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

3,551,987 A	1/1971	Wilkinson
4,773,420 A	9/1988	Green
4,844,068 A	7/1989	Arata et al.
4,903,697 A	2/1990	Resnick et al.
5,074,454 A	12/1991	Peters
5,405,072 A	4/1995	Zlock et al.
5,413,272 A	5/1995	Green et al.
5,415,334 A	5/1995	Williamson, IV et al.

OTHER PUBLICATIONS

Datasheet for Panasonic TK Relays Ultra Low Profile 2 A Polarized
Relay, Copyright Matsushita Electric Works, Ltd. (Known of at least
as early as Aug. 17, 2010), 5 pages.


(Continued)

Primary Examiner — Michelle Lopez

(57) **ABSTRACT**

Various embodiments are directed to a powered surgical
instrument for cutting and fastening tissue. The instrument
may comprise an end effector comprising a first jaw member
and a second jaw member, a drive device, a clamping trigger,
and a control circuit. The control circuit may comprise a
power supply, a firing switch, a clamp switch, a switching
device and an end-of-stroke switch. The firing switch may be
electrically connected to, upon actuation, connect the power
supply to the drive device via a first connection comprising
the switching device and the firing switch.

19 Claims, 43 Drawing Sheets

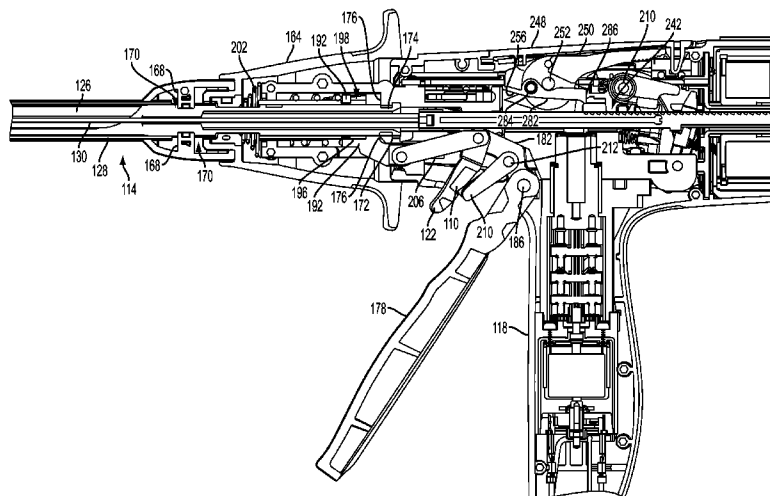

(56)

References Cited

U.S. PATENT DOCUMENTS

5,577,654 A	11/1996	Bishop	7,448,525 B2	11/2008	Shelton, IV et al.
5,588,579 A	12/1996	Schnut et al.	7,455,208 B2	11/2008	Wales et al.
5,601,224 A	2/1997	Bishop et al.	7,464,846 B2	12/2008	Shelton, IV et al.
5,603,443 A	2/1997	Clark et al.	7,464,849 B2	12/2008	Shelton, IV et al.
5,607,094 A	3/1997	Clark et al.	7,467,740 B2	12/2008	Shelton, IV et al.
5,628,446 A	5/1997	Geiste et al.	7,472,815 B2	1/2009	Shelton, IV et al.
5,630,539 A	5/1997	Plyley et al.	7,481,347 B2	1/2009	Roy
5,639,008 A	6/1997	Gallagher et al.	7,490,749 B2	2/2009	Schall et al.
5,651,491 A	7/1997	Heaton et al.	7,500,979 B2	3/2009	Hueil et al.
5,653,373 A	8/1997	Green et al.	7,506,791 B2	3/2009	Omaits et al.
5,662,258 A	9/1997	Knodel et al.	7,510,107 B2	3/2009	Timm et al.
5,673,840 A	10/1997	Schulze et al.	7,549,563 B2	6/2009	Mather et al.
5,673,841 A	10/1997	Schulze et al.	7,549,564 B2	6/2009	Boudreaux
5,680,981 A	10/1997	Millili et al.	7,556,185 B2	7/2009	Viola
5,680,982 A	10/1997	Schulze et al.	7,559,450 B2	7/2009	Wales et al.
5,692,668 A	12/1997	Schulze et al.	7,559,452 B2	7/2009	Wales et al.
5,704,534 A	1/1998	Huitema et al.	7,568,603 B2	8/2009	Shelton, IV et al.
5,711,472 A	1/1998	Bryan	7,568,604 B2	8/2009	Ehrenfels et al.
5,715,987 A	2/1998	Kelley et al.	7,575,144 B2	8/2009	Ortiz et al.
5,732,871 A	3/1998	Clark et al.	7,588,175 B2	9/2009	Timm et al.
5,797,536 A	8/1998	Smith et al.	7,588,176 B2	9/2009	Timm et al.
5,836,503 A	11/1998	Ehrenfels et al.	7,597,229 B2	10/2009	Boudreaux et al.
5,839,639 A	11/1998	Sauer et al.	7,604,150 B2	10/2009	Boudreaux
5,871,135 A	2/1999	Williamson, IV et al.	7,604,151 B2	10/2009	Hess et al.
5,941,442 A	8/1999	Geiste et al.	7,607,557 B2	10/2009	Shelton, IV et al.
6,241,139 B1	6/2001	Milliman et al.	7,624,902 B2	12/2009	Marczyk et al.
6,250,532 B1	6/2001	Green et al.	7,631,793 B2	12/2009	Rethy et al.
6,488,196 B1	12/2002	Fenton, Jr.	7,637,409 B2	12/2009	Marczyk
6,679,410 B2	1/2004	Würsch et al.	7,644,848 B2	1/2010	Swayze et al.
6,722,552 B2	4/2004	Fenton, Jr.	7,658,311 B2	2/2010	Boudreaux
6,755,338 B2	6/2004	Hahnen et al.	7,658,312 B2	2/2010	Vidal et al.
6,786,382 B1	9/2004	Hoffman	7,665,646 B2	2/2010	Prommersberger
6,830,174 B2	12/2004	Hillstead et al.	7,665,647 B2	2/2010	Shelton, IV et al.
6,866,178 B2	3/2005	Adams et al.	7,669,746 B2	3/2010	Shelton, IV
6,874,669 B2	4/2005	Adams et al.	7,669,747 B2	3/2010	Weisenburgh, II et al.
6,945,444 B2	9/2005	Gresham et al.	7,670,334 B2	3/2010	Hueil et al.
6,953,138 B1	10/2005	Dworak et al.	7,673,780 B2	3/2010	Shelton, IV et al.
6,953,139 B2	10/2005	Milliman et al.	7,673,781 B2	3/2010	Swayze et al.
6,959,851 B2	11/2005	Heinrich	7,673,782 B2	3/2010	Hess et al.
6,964,363 B2	11/2005	Wales et al.	7,673,783 B2	3/2010	Morgan et al.
6,978,921 B2	12/2005	Shelton, IV et al.	7,699,204 B2	4/2010	Viola
6,981,628 B2	1/2006	Wales	7,708,180 B2	5/2010	Murray et al.
7,032,798 B2	4/2006	Whitman et al.	7,717,312 B2	5/2010	Beetel
7,032,799 B2	4/2006	Viola et al.	7,721,931 B2	5/2010	Shelton, IV et al.
7,044,352 B2	5/2006	Shelton, IV et al.	7,721,934 B2	5/2010	Shelton, IV et al.
7,111,769 B2	9/2006	Wales et al.	7,721,936 B2	5/2010	Shelton, IV et al.
7,140,527 B2	11/2006	Ehrenfels et al.	7,726,537 B2	6/2010	Olson et al.
7,182,239 B1	2/2007	Myers	7,731,072 B2	6/2010	Timm et al.
7,237,708 B1	7/2007	Guy et al.	7,735,703 B2	6/2010	Morgan et al.
7,246,734 B2	7/2007	Shelton, IV	7,738,971 B2	6/2010	Swayze et al.
7,303,106 B2	12/2007	Milliman et al.	7,740,159 B2	6/2010	Shelton, IV et al.
7,303,108 B2	12/2007	Shelton, IV	7,753,245 B2	7/2010	Boudreaux et al.
7,328,828 B2	2/2008	Ortiz et al.	7,753,904 B2	7/2010	Shelton, IV et al.
7,334,717 B2	2/2008	Rethy et al.	7,766,209 B2	8/2010	Baxter, III et al.
7,334,718 B2	2/2008	McAlister et al.	7,766,210 B2	8/2010	Shelton, IV et al.
7,354,447 B2	4/2008	Shelton, IV et al.	7,770,775 B2	8/2010	Shelton, IV et al.
7,357,287 B2	4/2008	Shelton, IV et al.	7,780,054 B2	8/2010	Wales
7,364,060 B2	4/2008	Milliman	7,784,662 B2	8/2010	Wales et al.
7,380,695 B2	6/2008	Doll et al.	7,793,812 B2	9/2010	Moore et al.
7,380,696 B2	6/2008	Shelton, IV et al.	7,794,475 B2	9/2010	Hess et al.
7,404,508 B2	7/2008	Smith et al.	7,798,386 B2	9/2010	Schall et al.
7,407,075 B2	8/2008	Holsten et al.	7,799,039 B2	9/2010	Shelton, IV et al.
7,407,076 B2	8/2008	Racenet et al.	7,810,692 B2	10/2010	Hall et al.
7,407,078 B2	8/2008	Shelton, IV et al.	7,810,693 B2	10/2010	Broehl et al.
7,410,086 B2	8/2008	Ortiz et al.	7,819,296 B2	10/2010	Hueil et al.
7,416,101 B2	8/2008	Shelton, IV et al.	7,819,297 B2	10/2010	Doll et al.
7,419,080 B2	9/2008	Smith et al.	7,819,298 B2	10/2010	Hall et al.
7,422,136 B1 *	9/2008	Marczyk 227/175.1	7,819,299 B2	10/2010	Shelton, IV et al.
7,422,139 B2	9/2008	Shelton, IV et al.	7,832,408 B2	11/2010	Shelton, IV et al.
7,431,188 B1	10/2008	Marczyk	7,832,611 B2	11/2010	Boyden et al.
7,431,189 B2	10/2008	Shelton, IV et al.	7,832,612 B2	11/2010	Baxter, III et al.
7,434,717 B2	10/2008	Shelton, IV et al.	7,837,080 B2	11/2010	Schwemberger
7,438,209 B1	10/2008	Hess et al.	7,845,537 B2	12/2010	Shelton, IV et al.
7,441,684 B2	10/2008	Shelton, IV et al.	7,857,185 B2	12/2010	Swayze et al.
7,441,685 B1	10/2008	Boudreaux	7,857,186 B2	12/2010	Baxter, III et al.
			7,861,906 B2	1/2011	Doll et al.
			7,866,527 B2	1/2011	Hall et al.
			7,891,531 B1	2/2011	Ward
			7,900,805 B2	3/2011	Shelton, IV et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

7,905,380 B2	3/2011	Shelton, IV et al.	2008/0169329 A1	7/2008	Shelton et al.
7,905,381 B2	3/2011	Baxter, III et al.	2008/0169330 A1	7/2008	Shelton et al.
7,909,221 B2	3/2011	Viola et al.	2008/0169331 A1	7/2008	Shelton et al.
7,913,891 B2	3/2011	Doll et al.	2008/0169332 A1	7/2008	Shelton et al.
7,918,376 B1	4/2011	Knodel et al.	2008/0169333 A1	7/2008	Shelton et al.
7,918,377 B2	4/2011	Measamer et al.	2008/0237296 A1	10/2008	Boudreaux et al.
7,922,061 B2	4/2011	Shelton, IV et al.	2008/0251568 A1	10/2008	Zemlok et al.
7,934,630 B2	5/2011	Shelton, IV et al.	2008/0251569 A1	10/2008	Smith et al.
7,950,560 B2	5/2011	Zemlok et al.	2008/0283570 A1	11/2008	Boyden et al.
7,954,682 B2	6/2011	Giordano et al.	2008/0296346 A1	12/2008	Shelton, IV et al.
7,954,684 B2	6/2011	Boudreaux	2008/0300580 A1	12/2008	Shelton, IV et al.
7,954,686 B2	6/2011	Baxter, III et al.	2008/0308602 A1	12/2008	Timm et al.
7,959,051 B2	6/2011	Smith et al.	2008/0308603 A1	12/2008	Shelton, IV et al.
7,966,799 B2	6/2011	Morgan et al.	2008/0314960 A1	12/2008	Marczyk et al.
7,967,180 B2	6/2011	Scirica	2009/0001121 A1	1/2009	Hess et al.
8,006,885 B2	8/2011	Marczyk	2009/0001124 A1	1/2009	Hess et al.
8,011,550 B2	9/2011	Aranyi et al.	2009/0001130 A1	1/2009	Hess et al.
8,011,551 B2	9/2011	Marczyk et al.	2009/0005807 A1	1/2009	Hess et al.
8,020,742 B2	9/2011	Marczyk	2009/0005808 A1	1/2009	Hess et al.
8,028,883 B2	10/2011	Stopek	2009/0005809 A1	1/2009	Hess et al.
D650,074 S	12/2011	Hunt et al.	2009/0012556 A1	1/2009	Boudreaux et al.
8,083,119 B2	12/2011	Prommersberger	2009/0076534 A1	3/2009	Shelton, IV et al.
8,091,756 B2	1/2012	Viola	2009/0078736 A1	3/2009	Van Lue
8,100,310 B2	1/2012	Zemlok	2009/0108048 A1	4/2009	Zemlok et al.
8,157,153 B2	4/2012	Shelton, IV et al.	2009/0149871 A9	6/2009	Kagan et al.
8,205,781 B2	6/2012	Baxter, III et al.	2009/0206125 A1	8/2009	Huitema et al.
8,210,415 B2	7/2012	Ward	2009/0206126 A1	8/2009	Huitema et al.
8,256,654 B2	9/2012	Bettuchi et al.	2009/0206131 A1	8/2009	Weisenburgh, II et al.
8,267,300 B2	9/2012	Boudreaux	2009/0206132 A1	8/2009	Hueil et al.
8,292,155 B2	10/2012	Shelton, IV et al.	2009/0206133 A1	8/2009	Morgan et al.
8,333,313 B2	12/2012	Boudreaux et al.	2009/0206137 A1	8/2009	Hall et al.
8,360,296 B2	1/2013	Zingman	2009/0206139 A1	8/2009	Hall et al.
8,393,514 B2	3/2013	Shelton, IV et al.	2009/0206140 A1	8/2009	Scheib et al.
8,453,914 B2	6/2013	Laurent et al.	2009/0206141 A1	8/2009	Huitema et al.
8,459,525 B2	6/2013	Yates et al.	2009/0206142 A1	8/2009	Huitema et al.
2005/0103819 A1	5/2005	Racenet et al.	2009/0206143 A1	8/2009	Huitema et al.
2005/0274768 A1	12/2005	Cummins et al.	2009/0209946 A1	8/2009	Swayze et al.
2006/0049229 A1	3/2006	Milliman et al.	2009/0209979 A1	8/2009	Yates et al.
2006/0201989 A1	9/2006	Ojeda	2009/0209990 A1	8/2009	Yates et al.
2006/0226196 A1	10/2006	Hueil et al.	2009/0242610 A1	10/2009	Shelton, IV et al.
2007/0023476 A1	2/2007	Whitman et al.	2009/0255975 A1	10/2009	Zemlok et al.
2007/0023477 A1	2/2007	Whitman et al.	2009/0255976 A1	10/2009	Marczyk et al.
2007/0102472 A1	5/2007	Shelton, IV	2009/0255977 A1	10/2009	Zemlok
2007/0106317 A1	5/2007	Shelton, IV et al.	2010/0032470 A1	2/2010	Hess et al.
2007/0114261 A1	5/2007	Ortiz et al.	2010/0065605 A1	3/2010	Shelton, IV et al.
2007/0175949 A1	8/2007	Shelton, IV et al.	2010/0069942 A1	3/2010	Shelton, IV
2007/0175950 A1	8/2007	Shelton, IV et al.	2010/0076474 A1	3/2010	Yates et al.
2007/0175951 A1	8/2007	Shelton, IV et al.	2010/0076475 A1	3/2010	Yates et al.
2007/0175953 A1	8/2007	Shelton, IV et al.	2010/0089970 A1	4/2010	Smith et al.
2007/0175955 A1	8/2007	Shelton, IV et al.	2010/0089974 A1	4/2010	Shelton, IV
2007/0175956 A1*	8/2007	Swayze et al. 227/178.1	2010/0108740 A1	5/2010	Pastorelli et al.
2007/0194079 A1	8/2007	Hueil et al.	2010/0127042 A1	5/2010	Shelton, IV
2007/0194081 A1	8/2007	Hueil et al.	2010/0133317 A1	6/2010	Shelton, IV et al.
2007/0194082 A1	8/2007	Morgan et al.	2010/0133318 A1	6/2010	Boudreaux
2007/0221700 A1	9/2007	Ortiz et al.	2010/0179382 A1	7/2010	Shelton, IV et al.
2007/0221701 A1	9/2007	Ortiz et al.	2010/0181364 A1	7/2010	Shelton, IV et al.
2007/0225562 A1	9/2007	Spivey et al.	2010/0193566 A1	8/2010	Schieb et al.
2007/0239028 A1	10/2007	Houser et al.	2010/0193567 A1	8/2010	Scheib et al.
2007/0246505 A1	10/2007	Pace-Florida et al.	2010/0193568 A1	8/2010	Scheib et al.
2007/0295780 A1	12/2007	Shelton et al.	2010/0193569 A1	8/2010	Yates et al.
2008/0029570 A1	2/2008	Shelton et al.	2010/0198220 A1	8/2010	Boudreaux et al.
2008/0029573 A1	2/2008	Shelton et al.	2010/0200637 A1	8/2010	Beetel
2008/0029574 A1	2/2008	Shelton et al.	2010/0213241 A1	8/2010	Bedi et al.
2008/0029575 A1	2/2008	Shelton et al.	2010/0222901 A1	9/2010	Swayze et al.
2008/0078800 A1	4/2008	Hess et al.	2010/0224669 A1	9/2010	Shelton, IV et al.
2008/0078802 A1	4/2008	Hess et al.	2010/0237132 A1	9/2010	Measamer et al.
2008/0078803 A1	4/2008	Shelton et al.	2010/0243709 A1	9/2010	Hess et al.
2008/0078804 A1	4/2008	Shelton et al.	2010/0258611 A1	10/2010	Smith et al.
2008/0078806 A1	4/2008	Omaits et al.	2010/0264193 A1	10/2010	Huang et al.
2008/0078807 A1	4/2008	Hess et al.	2010/0264194 A1	10/2010	Huang et al.
2008/0078808 A1	4/2008	Hess et al.	2010/0294827 A1	11/2010	Boyden et al.
2008/0082125 A1	4/2008	Murray et al.	2010/0294829 A1	11/2010	Giordano et al.
2008/0167522 A1	7/2008	Giordano et al.	2010/0301095 A1	12/2010	Shelton, IV et al.
2008/0167672 A1	7/2008	Giordano et al.	2010/0301096 A1	12/2010	Moore et al.
2008/0169328 A1	7/2008	Shelton	2010/0305552 A1	12/2010	Shelton, IV et al.
			2010/0308100 A1	12/2010	Boudreaux
			2011/0006099 A1	1/2011	Hall et al.
			2011/0006101 A1	1/2011	Hall et al.
			2011/0006103 A1	1/2011	Laurent et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2011/0011914 A1	1/2011	Baxter, III et al.	2012/0080340 A1	4/2012	Shelton, IV et al.
2011/0011915 A1	1/2011	Shelton, IV	2012/0080344 A1	4/2012	Shelton, IV
2011/0017801 A1	1/2011	Zemlok et al.	2012/0080345 A1	4/2012	Morgan et al.
2011/0024477 A1	2/2011	Hall	2012/0080475 A1	4/2012	Smith et al.
2011/0024478 A1	2/2011	Shelton, IV	2012/0080478 A1	4/2012	Morgan et al.
2011/0024479 A1	2/2011	Swensgard et al.	2012/0080479 A1	4/2012	Shelton, IV
2011/0036887 A1	2/2011	Zemlok et al.	2012/0080480 A1	4/2012	Woodard, Jr. et al.
2011/0042441 A1	2/2011	Shelton, IV et al.	2012/0080481 A1	4/2012	Widenhouse et al.
2011/0060363 A1	3/2011	Hess et al.	2012/0080482 A1	4/2012	Schall et al.
2011/0062212 A1	3/2011	Shelton, IV et al.	2012/0080483 A1	4/2012	Riestenberg et al.
2011/0068145 A1	3/2011	Bedi et al.	2012/0080484 A1	4/2012	Morgan et al.
2011/0068148 A1	3/2011	Hall et al.	2012/0080485 A1	4/2012	Woodard, Jr. et al.
2011/0084113 A1	4/2011	Bedi et al.	2012/0080486 A1	4/2012	Woodard, Jr. et al.
2011/0084115 A1	4/2011	Bedi et al.	2012/0080487 A1	4/2012	Woodard, Jr. et al.
2011/0087276 A1	4/2011	Bedi et al.	2012/0080488 A1	4/2012	Shelton, IV et al.
2011/0101065 A1	5/2011	Milliman	2012/0080489 A1	4/2012	Shelton, IV et al.
2011/0114697 A1	5/2011	Baxter, III et al.	2012/0080490 A1	4/2012	Shelton, IV et al.
2011/0114698 A1	5/2011	Baxter, III et al.	2012/0080491 A1	4/2012	Shelton, IV et al.
2011/0114699 A1	5/2011	Baxter, III et al.	2012/0080493 A1	4/2012	Shelton, IV et al.
2011/0114700 A1	5/2011	Baxter, III et al.	2012/0080496 A1	4/2012	Schall et al.
2011/0118761 A1	5/2011	Baxter, III et al.	2012/0080498 A1	4/2012	Shelton, IV et al.
2011/0121051 A1	5/2011	Shelton, IV et al.	2012/0080499 A1	4/2012	Schall et al.
2011/0121052 A1	5/2011	Shelton, IV et al.	2012/0080500 A1	4/2012	Morgan et al.
2011/0125176 A1	5/2011	Yates et al.	2012/0080501 A1	4/2012	Morgan et al.
2011/0125177 A1	5/2011	Yates et al.	2012/0080502 A1	4/2012	Morgan et al.
2011/0132962 A1	6/2011	Hall et al.	2012/0080503 A1	4/2012	Woodard, Jr. et al.
2011/0132963 A1	6/2011	Giordano et al.	2012/0083833 A1	4/2012	Shelton, IV et al.
2011/0132964 A1	6/2011	Weisenburgh, II et al.	2012/0083834 A1	4/2012	Shelton, IV et al.
2011/0132965 A1	6/2011	Moore et al.	2012/0083835 A1	4/2012	Shelton, IV et al.
2011/0139852 A1	6/2011	Zingman	2012/0083836 A1	4/2012	Shelton, IV et al.
2011/0144430 A1	6/2011	Spivey et al.	2012/0132450 A1	5/2012	Timm et al.
2011/0147433 A1	6/2011	Shelton, IV et al.	2012/0138658 A1	6/2012	Ullrich et al.
2011/0147434 A1	6/2011	Hueil et al.	2012/0138660 A1	6/2012	Shelton, IV
2011/0155780 A1	6/2011	Boudreaux	2012/0160721 A1	6/2012	Shelton, IV et al.
2011/0155781 A1	6/2011	Swensgard et al.	2012/0175399 A1	7/2012	Shelton et al.
2011/0155785 A1	6/2011	Laurent et al.	2012/0199630 A1	8/2012	Shelton, IV et al.
2011/0155787 A1	6/2011	Baxter, III et al.	2012/0199631 A1	8/2012	Shelton, IV et al.
2011/0163147 A1	7/2011	Laurent et al.	2012/0199632 A1	8/2012	Spivey et al.
2011/0174861 A1	7/2011	Shelton, IV et al.	2012/0199633 A1	8/2012	Shelton, IV et al.
2011/0174863 A1	7/2011	Shelton, IV et al.	2012/0203247 A1	8/2012	Shelton, IV et al.
2011/0192882 A1	8/2011	Hess et al.	2012/0205421 A1	8/2012	Shelton, IV
2011/0210156 A1	9/2011	Smith et al.	2012/0211546 A1	8/2012	Shelton, IV
2011/0226837 A1	9/2011	Baxter, III et al.	2012/0234890 A1	9/2012	Aronhalt et al.
2011/0253765 A1	10/2011	Nicholas et al.	2012/0234891 A1	9/2012	Aronhalt et al.
2011/0275901 A1	11/2011	Shelton, IV	2012/0234892 A1	9/2012	Aronhalt et al.
2011/0276083 A1	11/2011	Shelton, IV et al.	2012/0234893 A1	9/2012	Schuckmann et al.
2011/0288573 A1	11/2011	Yates et al.	2012/0234895 A1	9/2012	O'Connor et al.
2011/0290851 A1	12/2011	Shelton, IV	2012/0234896 A1	9/2012	Ellerhorst et al.
2011/0290853 A1	12/2011	Shelton, IV et al.	2012/0234897 A1	9/2012	Shelton, IV et al.
2011/0290854 A1	12/2011	Timm et al.	2012/0234898 A1	9/2012	Shelton, IV et al.
2011/0290855 A1	12/2011	Moore et al.	2012/0234899 A1	9/2012	Scheib et al.
2011/0290856 A1	12/2011	Shelton, IV et al.	2012/0234900 A1	9/2012	Swayze
2011/0295242 A1	12/2011	Spivey et al.	2012/0238823 A1	9/2012	Hagerty et al.
2011/0295269 A1	12/2011	Swensgard et al.	2012/0238824 A1	9/2012	Widenhouse et al.
2011/0295270 A1	12/2011	Giordano et al.	2012/0238826 A1	9/2012	Yoo et al.
2011/0295295 A1	12/2011	Shelton, IV et al.	2012/0238829 A1	9/2012	Shelton, IV et al.
2012/0024934 A1	2/2012	Shelton, IV et al.	2012/0239009 A1	9/2012	Mollere et al.
2012/0024935 A1	2/2012	Shelton, IV et al.	2012/0239010 A1	9/2012	Shelton, IV et al.
2012/0024936 A1	2/2012	Baxter, III et al.	2012/0239075 A1	9/2012	Widenhouse et al.
2012/0029272 A1	2/2012	Shelton, IV et al.	2012/0239082 A1	9/2012	Shelton, IV et al.
2012/0029544 A1	2/2012	Shelton, IV et al.	2012/0241491 A1	9/2012	Aldridge et al.
2012/0029547 A1	2/2012	Shelton, IV et al.	2012/0241492 A1	9/2012	Shelton, IV et al.
2012/0071711 A1	3/2012	Shelton, IV et al.	2012/0241493 A1	9/2012	Baxter, III et al.
2012/0071866 A1	3/2012	Kerr et al.	2012/0241496 A1	9/2012	Mandakolathur Vasudevan et al.
2012/0074196 A1	3/2012	Shelton, IV et al.	2012/0241497 A1	9/2012	Mandakolathur Vasudevan et al.
2012/0074198 A1	3/2012	Huitema et al.	2012/0241498 A1	9/2012	Gonzalez et al.
2012/0074200 A1	3/2012	Schmid et al.	2012/0241499 A1	9/2012	Baxter, III et al.
2012/0074201 A1	3/2012	Baxter, III et al.	2012/0241500 A1	9/2012	Timmer et al.
2012/0080332 A1	4/2012	Shelton, IV et al.	2012/0241501 A1	9/2012	Swayze et al.
2012/0080333 A1	4/2012	Woodard, Jr. et al.	2012/0241502 A1	9/2012	Aldridge et al.
2012/0080335 A1	4/2012	Shelton, IV et al.	2012/0241503 A1	9/2012	Baxter, III et al.
2012/0080336 A1	4/2012	Shelton, IV et al.	2012/0241505 A1	9/2012	Alexander, III et al.
2012/0080337 A1	4/2012	Shelton, IV et al.	2012/0248169 A1	10/2012	Widenhouse et al.
2012/0080338 A1	4/2012	Shelton, IV et al.	2012/0253298 A1	10/2012	Henderson et al.
2012/0080339 A1	4/2012	Shelton, IV et al.	2012/0265230 A1	10/2012	Yates et al.
			2012/0273551 A1	11/2012	Shelton, IV et al.
			2012/0283707 A1	11/2012	Giordano et al.
			2012/0283748 A1	11/2012	Ortiz et al.
			2012/0286019 A1	11/2012	Hueil et al.

(56)

References Cited**U.S. PATENT DOCUMENTS**

2012/0292367 A1 11/2012 Morgan et al.
 2012/0292370 A1 11/2012 Hess et al.
 2012/0298719 A1 11/2012 Shelton, IV et al.
 2013/0012931 A1 1/2013 Spivey et al.
 2013/0012957 A1 1/2013 Shelton, IV et al.
 2013/0020376 A1 1/2013 Shelton, IV et al.
 2013/0023861 A1 1/2013 Shelton, IV et al.
 2013/0026208 A1 1/2013 Shelton, IV et al.
 2013/0026210 A1 1/2013 Shelton, IV et al.
 2013/0056518 A1 3/2013 Swensgard
 2013/0056520 A1 3/2013 Swensgard
 2013/0056521 A1 3/2013 Swensgard
 2013/0056522 A1 3/2013 Swensgard
 2013/0075443 A1 3/2013 Giordano et al.
 2013/0075448 A1 3/2013 Schmid et al.
 2013/0075449 A1 3/2013 Schmid et al.
 2013/0075450 A1 3/2013 Schmid et al.
 2013/0105551 A1 5/2013 Zingman
 2013/0126581 A1 5/2013 Yates et al.
 2013/0126582 A1 5/2013 Shelton, IV et al.
 2013/0126583 A1 5/2013 Hueil et al.
 2013/0146641 A1 6/2013 Shelton, IV et al.
 2013/0146642 A1 6/2013 Shelton, IV et al.
 2013/0146643 A1 6/2013 Schmid et al.
 2013/0153636 A1 6/2013 Shelton, IV et al.
 2013/0153641 A1 6/2013 Shelton, IV et al.

FOREIGN PATENT DOCUMENTS

CA 2514274 A1 1/2006
 CN 2488482 Y 5/2002
 CN 1634601 A 7/2005
 CN 1868411 A 11/2006
 CN 1915180 A 2/2007
 CN 101011286 A 8/2007
 CN 101095621 A 1/2008
 DE 273689 C 5/1914
 DE 1775926 A 1/1972
 DE 3210466 A1 9/1983
 DE 3709067 A1 9/1988
 DE 9412228 U 9/1994
 DE 19509116 A1 9/1996
 DE 19851291 A1 1/2000
 DE 19924311 A1 11/2000
 DE 69328576 T2 1/2001
 DE 10052679 A1 5/2001
 DE 20112837 U1 10/2001
 DE 20121753 U1 4/2003
 DE 10314072 A1 10/2004
 DE 202007003114 U1 6/2007
 EP 0122046 A1 10/1984
 EP 0070230 B1 10/1985
 EP 0156774 A2 10/1985
 EP 0387980 B1 10/1985
 EP 0033548 B1 5/1986
 EP 0129442 B1 11/1987
 EP 0276104 A2 7/1988
 EP 0178940 B1 1/1991
 EP 0178941 B1 1/1991
 EP 0248844 B1 1/1993
 EP 0545029 A1 6/1993
 EP 0277959 B1 10/1993
 EP 0233940 B1 11/1993
 EP 0261230 B1 11/1993
 EP 0639349 A2 2/1994
 EP 0324636 B1 3/1994
 EP 0593920 A1 4/1994
 EP 0594148 A1 4/1994
 EP 0427949 B1 6/1994
 EP 0523174 B1 6/1994
 EP 0600182 A2 6/1994
 EP 0310431 B1 11/1994
 EP 0375302 B1 11/1994
 EP 0376562 B1 11/1994

EP 0630612 A1 12/1994
 EP 0634144 A1 1/1995
 EP 0646356 A2 4/1995
 EP 0646357 A1 4/1995
 EP 0653189 A2 5/1995
 EP 0669104 A1 8/1995
 EP 0511470 B1 10/1995
 EP 0674876 A2 10/1995
 EP 0679367 A2 11/1995
 EP 0392547 B1 12/1995
 EP 0685204 A1 12/1995
 EP 0364216 B1 1/1996
 EP 0699418 A1 3/1996
 EP 0702937 A1 3/1996
 EP 0705571 A1 4/1996
 EP 0711611 A2 5/1996
 EP 0484677 B2 6/1996
 EP 0541987 B1 7/1996
 EP 0667119 B1 7/1996
 EP 0708618 B1 3/1997
 EP 0770355 A1 5/1997
 EP 0503662 B1 6/1997
 EP 0447121 B1 7/1997
 EP 0625077 B1 7/1997
 EP 0633749 B1 8/1997
 EP 0710090 B1 8/1997
 EP 0578425 B1 9/1997
 EP 0625335 B1 11/1997
 EP 0552423 B1 1/1998
 EP 0592244 B1 1/1998
 EP 0648476 B1 1/1998
 EP 0649290 B1 3/1998
 EP 0598618 B1 9/1998
 EP 0676173 B1 9/1998
 EP 0678007 B1 9/1998
 EP 0603472 B1 11/1998
 EP 0605351 B1 11/1998
 EP 0878169 A1 11/1998
 EP 0879742 A1 11/1998
 EP 0695144 B1 12/1998
 EP 0722296 B1 12/1998
 EP 0760230 B1 2/1999
 EP 0623316 B1 3/1999
 EP 0650701 B1 3/1999
 EP 0537572 B1 6/1999
 EP 0923907 A1 6/1999
 EP 0843906 B1 3/2000
 EP 0552050 B 5/2000
 EP 0833592 B1 5/2000
 EP 0830094 B1 9/2000
 EP 1034747 A1 9/2000
 EP 1034748 A1 9/2000
 EP 0694290 B1 11/2000
 EP 1050278 A1 11/2000
 EP 1053719 A1 11/2000
 EP 1053720 A1 11/2000
 EP 1055399 A1 11/2000
 EP 1055400 A1 11/2000
 EP 1080694 A1 3/2001
 EP 1090592 A1 4/2001
 EP 1095627 A1 5/2001
 EP 1256318 B1 5/2001
 EP 0806914 B1 9/2001
 EP 0768840 B1 12/2001
 EP 0908152 B1 1/2002
 EP 0872213 B1 5/2002
 EP 0862386 B1 6/2002
 EP 0949886 B1 9/2002
 EP 1238634 A2 9/2002
 EP 0858295 B1 12/2002
 EP 0656188 B1 1/2003
 EP 0717960 B1 2/2003
 EP 1284120 A1 2/2003
 EP 1287788 A1 3/2003
 EP 0717966 B1 4/2003
 EP 0869742 B1 5/2003
 EP 0829235 B1 6/2003
 EP 0887046 B1 7/2003
 EP 0852480 B1 8/2003

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	0891154	B1	9/2003	EP	1769756	A1	4/2007
EP	0813843	B1	10/2003	EP	1769758	A1	4/2007
EP	0873089	B1	10/2003	EP	1581128	B1	5/2007
EP	0856326	B1	11/2003	EP	1780825	A1	5/2007
EP	1374788	A1	1/2004	EP	1785097	A2	5/2007
EP	0741996	B1	2/2004	EP	1790293	A2	5/2007
EP	0814712	B1	2/2004	EP	1800610	A1	6/2007
EP	1402837	A1	3/2004	EP	1300117	B1	8/2007
EP	0705570	B1	4/2004	EP	1813199	A1	8/2007
EP	0959784	B1	4/2004	EP	1813201	A1	8/2007
EP	1407719	A2	4/2004	EP	1813202	A1	8/2007
EP	1086713	B1	5/2004	EP	1813203	A2	8/2007
EP	0996378	B1	6/2004	EP	1813207	A1	8/2007
EP	1426012	A1	6/2004	EP	1813209	A1	8/2007
EP	0833593	B2	7/2004	EP	1487359	B1	10/2007
EP	1442694	A1	8/2004	EP	1599146	B1	10/2007
EP	0888749	B1	9/2004	EP	1839596	A1	10/2007
EP	0959786	B1	9/2004	EP	2110083	A2	10/2007
EP	1459695	A1	9/2004	EP	1857057	A2	11/2007
EP	1254636	B1	10/2004	EP	1402821	B1	12/2007
EP	1473819	A1	11/2004	EP	1872727	A1	1/2008
EP	1477119	A1	11/2004	EP	1897502	A1	3/2008
EP	1479345	A1	11/2004	EP	1908417	A2	4/2008
EP	1479347	A1	11/2004	EP	1330201	B1	6/2008
EP	1479348	A1	11/2004	EP	1702568	B1	7/2008
EP	0754437	B2	12/2004	EP	1943955	A2	7/2008
EP	1025807	B1	12/2004	EP	1943957	A2	7/2008
EP	1001710	B1	1/2005	EP	1943964	A1	7/2008
EP	1520521	A1	4/2005	EP	1943976	A2	7/2008
EP	1520522	A1	4/2005	EP	1593337	B1	8/2008
EP	1520523	A1	4/2005	EP	1970014	A1	9/2008
EP	1520525	A1	4/2005	EP	1980213	A2	10/2008
EP	1522264	A1	4/2005	EP	1759645	B1	11/2008
EP	1523942	A2	4/2005	EP	1990014	A2	11/2008
EP	1550408	A1	7/2005	EP	1693008	B1	12/2008
EP	1557129	A1	7/2005	EP	1759640	B1	12/2008
EP	1064883	B1	8/2005	EP	2000102	A2	12/2008
EP	1067876	B1	8/2005	EP	2005894	A2	12/2008
EP	0870473	B1	9/2005	EP	2008595	A2	12/2008
EP	1157666	B1	9/2005	EP	1736104	B1	3/2009
EP	0880338	B1	10/2005	EP	1749486	B1	3/2009
EP	1158917	B1	11/2005	EP	2039316	A2	3/2009
EP	1344498	B1	11/2005	EP	1721576	B1	4/2009
EP	1330989	B1	12/2005	EP	1733686	B1	4/2009
EP	0771176	B2	1/2006	EP	2044890	A1	4/2009
EP	1621138	A2	2/2006	EP	1550409	A1	6/2009
EP	1621139	A2	2/2006	EP	1550413	B1	6/2009
EP	1621141	A2	2/2006	EP	1745748	B1	8/2009
EP	1621145	A2	2/2006	EP	2090237	A1	8/2009
EP	1621151	A2	2/2006	EP	2090241	A1	8/2009
EP	1034746	B1	3/2006	EP	2090244	A2	8/2009
EP	1632191	A2	3/2006	EP	2090245	A1	8/2009
EP	1065981	B1	5/2006	EP	2090256	A2	8/2009
EP	1082944	B1	5/2006	EP	2095777	A2	9/2009
EP	1652481	A2	5/2006	EP	2098170	A2	9/2009
EP	1382303	B1	6/2006	EP	2110082	A1	10/2009
EP	1253866	B1	7/2006	EP	2111803	A2	10/2009
EP	1032318	B1	8/2006	EP	1813208	B1	11/2009
EP	1045672	B1	8/2006	EP	1908426	B1	11/2009
EP	1617768	B1	8/2006	EP	2116195	A1	11/2009
EP	1693015	A2	8/2006	EP	1607050	B1	12/2009
EP	1400214	B1	9/2006	EP	1815804	B1	12/2009
EP	1702567	A2	9/2006	EP	1566150	B1	4/2010
EP	1129665	B1	11/2006	EP	1813206	B1	4/2010
EP	1400206	B1	11/2006	EP	1769754	B1	6/2010
EP	1721568	A1	11/2006	EP	1854416	B1	6/2010
EP	1256317	B1	12/2006	EP	1535565	B1	10/2010
EP	1285633	B1	12/2006	EP	1702570	B1	10/2010
EP	1728473	A1	12/2006	EP	1785098	B1	10/2010
EP	1728475	A2	12/2006	EP	2005896	B1	10/2010
EP	1479346	B1	1/2007	EP	2030578	B1	11/2010
EP	1484024	B1	1/2007	EP	1627605	B1	12/2010
EP	1754445	A2	2/2007	EP	2286738	A2	2/2011
EP	1759812	A1	3/2007	EP	1690502	B1	3/2011
EP	1767163	A1	3/2007	EP	1769755	B1	4/2011
				EP	1813205	B1	6/2011
				EP	2090243	B1	6/2011
				EP	2329773	A1	6/2011
				EP	1908414	B1	11/2011

(56)

References Cited

FOREIGN PATENT DOCUMENTS

EP	1785102	B1	1/2012	RU	RU 2141279	C1	11/1999
EP	2090253	B1	3/2012	RU	2187249	C2	8/2002
EP	2005895	B1	8/2012	RU	2225170	C2	3/2004
EP	2090248	B1	8/2012	SU	189517	A	1/1967
EP	1884206	B1	3/2013	SU	328636	A	9/1972
FR	999646	A	2/1952	SU	886900	A1	12/1981
FR	1112936	A	3/1956	SU	1333319	A2	8/1987
FR	2598905	A1	11/1987	SU	1377053	A1	2/1988
FR	2765794	A	1/1999	SU	1561964	A1	5/1990
GB	939929	A	10/1963	SU	1722476	A1	3/1992
GB	1210522	A	10/1970	WO	WO 82/02824	A1	9/1982
GB	1217159	A	12/1970	WO	WO 91/15157	A1	10/1991
GB	1339394	A	12/1973	WO	WO 92/20295	A1	11/1992
GB	2109241	A	6/1983	WO	WO 92/21300	A1	12/1992
GB	2272159	A	5/1994	WO	WO 93/08755	A1	5/1993
GB	2284242	A	5/1995	WO	WO 93/13718	A1	7/1993
GB	2336214	A	10/1999	WO	WO 93/14690	A1	8/1993
GB	2425903	A	11/2006	WO	WO 93/15648	A1	8/1993
JP	S 58500053	A	1/1983	WO	WO 93/15850	A1	8/1993
JP	61-98249	A	5/1986	WO	WO 93/19681	A1	10/1993
JP	S 61502036	A	9/1986	WO	WO 94/00060	A1	1/1994
JP	S 63-147449	A	6/1988	WO	WO 94/11057	A1	5/1994
JP	63-203149	A	8/1988	WO	WO 94/12108	A1	6/1994
JP	3-12126	A	1/1991	WO	WO 94/18893	A1	9/1994
JP	5-212039	A	8/1993	WO	WO 94/22378	A1	10/1994
JP	6007357	A	1/1994	WO	WO 94/23659	A1	10/1994
JP	H 6-30945	A	2/1994	WO	WO 95/02369	A1	1/1995
JP	H 6-121798	A	5/1994	WO	WO 95/03743	A1	2/1995
JP	7051273	A	2/1995	WO	WO 95/06817	A1	3/1995
JP	7-124166	A	5/1995	WO	WO 95/09576	A1	4/1995
JP	7-255735	A	10/1995	WO	WO 95/09577	A1	4/1995
JP	8-33642	A	2/1996	WO	WO 95/14436	A1	6/1995
JP	8033641	A	2/1996	WO	WO 95/17855	A1	7/1995
JP	8-164141	A	6/1996	WO	WO 95/18383	A1	7/1995
JP	8229050	A	9/1996	WO	WO 95/18572	A1	7/1995
JP	H 09-501081	A	2/1997	WO	WO 95/19739	A1	7/1995
JP	2000-14632	A	1/2000	WO	WO 95/20360	A1	8/1995
JP	2000033071	A	2/2000	WO	WO 95/23557	A1	9/1995
JP	2000171730	A	6/2000	WO	WO 95/24865	A1	9/1995
JP	2000287987	A	10/2000	WO	WO 95/25471	A3	9/1995
JP	2000325303	A	11/2000	WO	WO 95/26562	A1	10/1995
JP	2001-514541	A	9/2001	WO	WO 95/29639	A1	11/1995
JP	2001-517473	A	10/2001	WO	WO 96/04858	A1	2/1996
JP	2001286477	A	10/2001	WO	WO 96/18344	A2	6/1996
JP	2002143078	A	5/2002	WO	WO 96/19151	A1	6/1996
JP	2002369820	A	12/2002	WO	WO 96/19152	A1	6/1996
JP	2003-500153	A	1/2003	WO	WO 96/20652	A1	7/1996
JP	2003-521301	A	7/2003	WO	WO 96/21119	A1	7/1996
JP	2004-162035	A	6/2004	WO	WO 96/22055	A1	7/1996
JP	2004-329624	A	11/2004	WO	WO 96/23448	A1	8/1996
JP	2004-344663	A	12/2004	WO	WO 96/24301	A1	8/1996
JP	2005-028147	A	2/2005	WO	WO 96/27337	A1	9/1996
JP	2005-028149	A	2/2005	WO	WO 96/31155	A1	10/1996
JP	2005-505309	A	2/2005	WO	WO 96/35464	A1	11/1996
JP	2005505322	T	2/2005	WO	WO 96/39085	A1	12/1996
JP	2005103293	A	4/2005	WO	WO 96/39086	A1	12/1996
JP	2005131163	A	5/2005	WO	WO 96/39087	A1	12/1996
JP	2005131164	A	5/2005	WO	WO 96/39088	A1	12/1996
JP	2005131173	A	5/2005	WO	WO 96/39089	A1	12/1996
JP	2005131211	A	5/2005	WO	WO 97/00646	A1	1/1997
JP	2005131212	A	5/2005	WO	WO 97/00647	A1	1/1997
JP	2005137423	A	6/2005	WO	WO 97/06582	A1	2/1997
JP	2005152416	A	6/2005	WO	WO 97/10763	A1	3/1997
JP	2005-523105	A	8/2005	WO	WO 97/10764	A1	3/1997
JP	2005524474	A	8/2005	WO	WO 97/11648	A2	4/1997
JP	2006-034975	A	2/2006	WO	WO 97/11649	A1	4/1997
JP	2006-034980	A	2/2006	WO	WO 97/15237	A1	5/1997
JP	2006-218297	A	8/2006	WO	WO 97/24073	A1	7/1997
JP	2006-281405	A	10/2006	WO	WO 97/24993	A1	7/1997
JP	2007-098130	A	4/2007	WO	WO 97/30644	A1	8/1997
JP	2007-117725	A	5/2007	WO	WO 97/34533	A1	9/1997
JP	2007-203057	A	8/2007	WO	WO 97/37598	A1	10/1997
JP	2007-229448	A	9/2007	WO	WO 97/39688	A2	10/1997
JP	2008-283459	A	11/2008	WO	WO 98/17180	A1	4/1998
RU	2008830	C1	3/1994	WO	WO 98/27880	A1	7/1998
				WO	WO 98/30153	A1	7/1998
				WO	WO 98/47436	A1	10/1998
				WO	WO 99/03407	A1	1/1999
				WO	WO 99/03408	A1	1/1999

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO 99/03409	A1	1/1999	WO	WO 03/101313	A1	12/2003
WO	WO 99/12483	A1	3/1999	WO	WO 03/105698	A2	12/2003
WO	WO 99/12487	A1	3/1999	WO	WO 03/105702	A2	12/2003
WO	WO 99/12488	A1	3/1999	WO	WO 2004/006980	A2	1/2004
WO	WO 99/15086	A1	4/1999	WO	WO 2004/011037	A2	2/2004
WO	WO 99/15091	A1	4/1999	WO	WO 2004/019769	A1	3/2004
WO	WO 99/23933	A2	5/1999	WO	WO 2004/021868	A2	3/2004
WO	WO 99/23959	A1	5/1999	WO	WO 2004/028585	A2	4/2004
WO	WO 99/25261	A1	5/1999	WO	WO 2004/032754	A2	4/2004
WO	WO 99/29244	A1	6/1999	WO	WO 2004/032760	A2	4/2004
WO	WO 99/34744	A1	7/1999	WO	WO 2004/032762	A1	4/2004
WO	WO 99/45849	A1	9/1999	WO	WO 2004/032763	A2	4/2004
WO	WO 99/48430	A1	9/1999	WO	WO 2004/034875	A2	4/2004
WO	WO 99/51158	A1	10/1999	WO	WO 2004/047626	A1	6/2004
WO	WO 00/24322	A1	5/2000	WO	WO 2004/047653	A2	6/2004
WO	WO 00/24330	A1	5/2000	WO	WO 2004/049956	A2	6/2004
WO	WO 00/41638	A1	7/2000	WO	WO 2004/052426	A2	6/2004
WO	WO 00/48506	A1	8/2000	WO	WO 2004/056276	A1	7/2004
WO	WO 00/53112	A2	9/2000	WO	WO 2004/056277	A1	7/2004
WO	WO 00/54653	A1	9/2000	WO	WO 2004/062516	A1	7/2004
WO	WO 00/057796	A1	10/2000	WO	WO 2004/078050	A2	9/2004
WO	WO 00/64365	A1	11/2000	WO	WO 2004/078051	A2	9/2004
WO	WO 00/72762	A1	12/2000	WO	WO 2004/086987	A1	10/2004
WO	WO 00/72765	A1	12/2000	WO	WO 2004/096015	A2	11/2004
WO	WO 01/03587	A1	1/2001	WO	WO 2004/096057	A2	11/2004
WO	WO 01/05702	A1	1/2001	WO	WO 2004/103157	A2	12/2004
WO	WO 01/010482	A1	2/2001	WO	WO 2004/105593	A1	12/2004
WO	WO 01/35845	A1	5/2001	WO	WO 2004/105621	A1	12/2004
WO	WO 01/54594	A1	8/2001	WO	WO 2004/112618	A2	12/2004
WO	WO 01/58371	A1	8/2001	WO	WO 2004/112652	A2	12/2004
WO	WO 01/62158	A2	8/2001	WO	WO 2005/027983	A2	3/2005
WO	WO 01/62161	A1	8/2001	WO	WO 2005/037329	A2	4/2005
WO	WO 01/62162	A1	8/2001	WO	WO 2005/044078	A2	5/2005
WO	WO 01/62164	A2	8/2001	WO	WO 2005/055846	A1	6/2005
WO	WO 01/62169	A2	8/2001	WO	WO 2005/072634	A2	8/2005
WO	WO 01/78605	A2	10/2001	WO	WO 2005/078892	A1	8/2005
WO	WO 01/91646	A1	12/2001	WO	WO 2005/079675	A2	9/2005
WO	WO 02/07608	A2	1/2002	WO	WO 2005/096954	A2	10/2005
WO	WO 02/07618	A1	1/2002	WO	WO 2005/112806	A2	12/2005
WO	WO 02/17799	A1	3/2002	WO	WO 2005/112808	A1	12/2005
WO	WO 02/19920	A1	3/2002	WO	WO 2005/115251	A2	12/2005
WO	WO 02/19932	A1	3/2002	WO	WO 2005/115253	A2	12/2005
WO	WO 02/30297	A2	4/2002	WO	WO 2005/117735	A1	12/2005
WO	WO 02/32322	A2	4/2002	WO	WO 2005/122936	A1	12/2005
WO	WO 02/36028	A1	5/2002	WO	WO 2006/023486	A1	3/2006
WO	WO 02/43571	A2	6/2002	WO	WO 2006/027014	A1	3/2006
WO	WO 02/058568	A1	8/2002	WO	WO 2006/044490	A2	4/2006
WO	WO 02/060328	A1	8/2002	WO	WO 2006/044581	A2	4/2006
WO	WO 02/067785	A2	9/2002	WO	WO 2006/044810	A2	4/2006
WO	WO 02/098302	A1	12/2002	WO	WO 2006/051252	A1	5/2006
WO	WO 03/000138	A2	1/2003	WO	WO 2006/059067	A1	6/2006
WO	WO 03/001329	A2	1/2003	WO	WO 2006/083748	A1	8/2006
WO	WO 03/013363	A1	2/2003	WO	WO 2006/092563	A1	9/2006
WO	WO 03/015604	A2	2/2003	WO	WO 2006/092565	A1	9/2006
WO	WO 03/020106	A2	3/2003	WO	WO 2006/115958	A1	11/2006
WO	WO 03/020139	A2	3/2003	WO	WO 2006/125940	A1	11/2006
WO	WO 03/024339	A1	3/2003	WO	WO 2006/132992	A1	12/2006
WO	WO 03/079909	A3	3/2003	WO	WO 2007/002180	A2	1/2007
WO	WO 03/030743	A2	4/2003	WO	WO 2007/016290	A2	2/2007
WO	WO 03/037193	A1	5/2003	WO	WO 2007/018898	A2	2/2007
WO	WO 03/047436	A3	6/2003	WO	WO 2007/098220	A2	8/2007
WO	WO 03/055402	A1	7/2003	WO	WO 2007/121579	A1	11/2007
WO	WO 03/057048	A1	7/2003	WO	WO 2007/131110	A2	11/2007
WO	WO 03/057058	A1	7/2003	WO	WO 2007/137304	A2	11/2007
WO	WO 03/063694	A1	8/2003	WO	WO 2007/139734	A2	12/2007
WO	WO 03/077769	A1	9/2003	WO	WO 2007/142625	A2	12/2007
WO	WO 03/079911	A1	10/2003	WO	WO 2007/147439	A1	12/2007
WO	WO 03/082126	A1	10/2003	WO	WO 2008/021969	A2	2/2008
WO	WO 03/086206	A1	10/2003	WO	WO 2008/039249	A1	4/2008
WO	WO 03/088845	A2	10/2003	WO	WO 2008/039270	A1	4/2008
WO	WO 03/090630	A2	11/2003	WO	WO 2008/045383	A2	4/2008
WO	WO 03/094743	A1	11/2003	WO	WO 2008/070763	A1	6/2008
WO	WO 03/094745	A1	11/2003	WO	WO 2008/089404	A2	7/2008
WO	WO 03/094746	A1	11/2003	WO	WO 2008/101080	A1	8/2008
WO	WO 03/094747	A1	11/2003	WO	WO 2008/109125	A1	9/2008
				WO	WO 2008/124748	A1	10/2008
				WO	WO 2009/046394	A1	4/2009
				WO	WO 2009/137761	A2	11/2009
				WO	WO 2010/030434	A1	3/2010

(56)

References Cited

FOREIGN PATENT DOCUMENTS

WO	WO 2010/063795	A1	6/2010
WO	WO 2010/098871	A2	9/2010
WO	WO 2012/021671	A1	2/2012
WO	WO 2012/044844	A2	4/2012

OTHER PUBLICATIONS

U.S. Appl. No. 12/884,838, filed Sep. 17, 2010, US PG Pub. 2012/0071711; Shelton, Frederick.

U.S. Appl. No. 12/884,995, filed Sep. 17, 2010, US PG Pub. 2012/0071866; Kerr, Wendy A.

Disclosed Anonymously, "Motor-Driven Surgical Stapler Improvements," Research Disclosure Database No. 526041, Published: Feb. 2008.

C.C. Thompson et al., "Peroral Endoscopic Reduction of Dilated Gastrojejunal Anastomosis After Roux-en-Y Gastric Bypass: A Possible New Option for Patients with Weight Regain," *Surg Endosc* (2006) vol. 20, pp. 1744-1748.

B.R. Coolman, DVM, MS et al., "Comparison of Skin Staples With Sutures for Anastomosis of the Small Intestine in Dogs," Abstract; <http://www.blackwell-synergy.com/doi/abs/10.1053/jvet.2000.7539?cookieSet=1&journalCode=vsu> which redirects to <http://www3.interscience.wiley.com/journal/119040681/abstract?CRETRY=1&SRETRY=0>; [online] accessed: Sep. 22, 2008 (2 pages).

The Soderm Aseptic Battery Transfer Kit, Soderm Systems, 2000, 3 pages.

The Soderm Aseptic Battery Transfer Kit, Soderm Systems, 2000, 3 pages.

"Biomedical Coatings," Fort Wayne Metals, Research Products Corporation, obtained online at www.fwmetals.com on Jun. 21, 2010 (1 page).

Van Meer et al., "A Disposable Plastic Compact Wrist for Smart Minimally Invasive Surgical Tools," LAAS/CNRS (Aug. 2005).

Breedveld et al., "A New, Easily Miniaturized Sterrable Endoscope," *IEEE Engineering in Medicine and Biology Magazine* (Nov./Dec. 2005).

D. Tuite, Ed., "Get the Lowdown on Ultracapacitors," Nov. 15, 2007; [online] URL: <http://electronicdesign.com/Articles/Print.cfm?ArticleID=17465>, accessed Jan. 15, 2008 (5 pages).

ASTM procedure D2240-00, "Standard Test Method for Rubber Property-Durometer Hardness," (Published Aug. 2000).

ASTM procedure D2240-05, "Standard Test Method for Rubber Property-Durometer Hardness," (Published Apr. 2010).

Covidien Brochure, "Endo GIA™ Reloads with Tri-Staple™ Technology," (2010), 1 page.

Covidien Brochure, "Endo GIA™ Reloads with Tri-Staple™ Technology and Endo GIA™ Ultra Universal Staplers," (2010), 2 pages.

Covidien Brochure, "Endo GIA™ Black Reload with Tri-Staple™ Technology," (2012), 2 pages.

Covidien Brochure, "Endo GIA™ Curved Tip Reload with Tri-Staple™ Technology," (2012), 2 pages.

Covidien Brochure, "Endo GIA™ Reloads with Tri-Stapler™ Technology," (2010), 2 pages.

Covidien Brochure, "Endo GIA™ Ultra Universal Stapler," (2010), 2 pages.

* cited by examiner

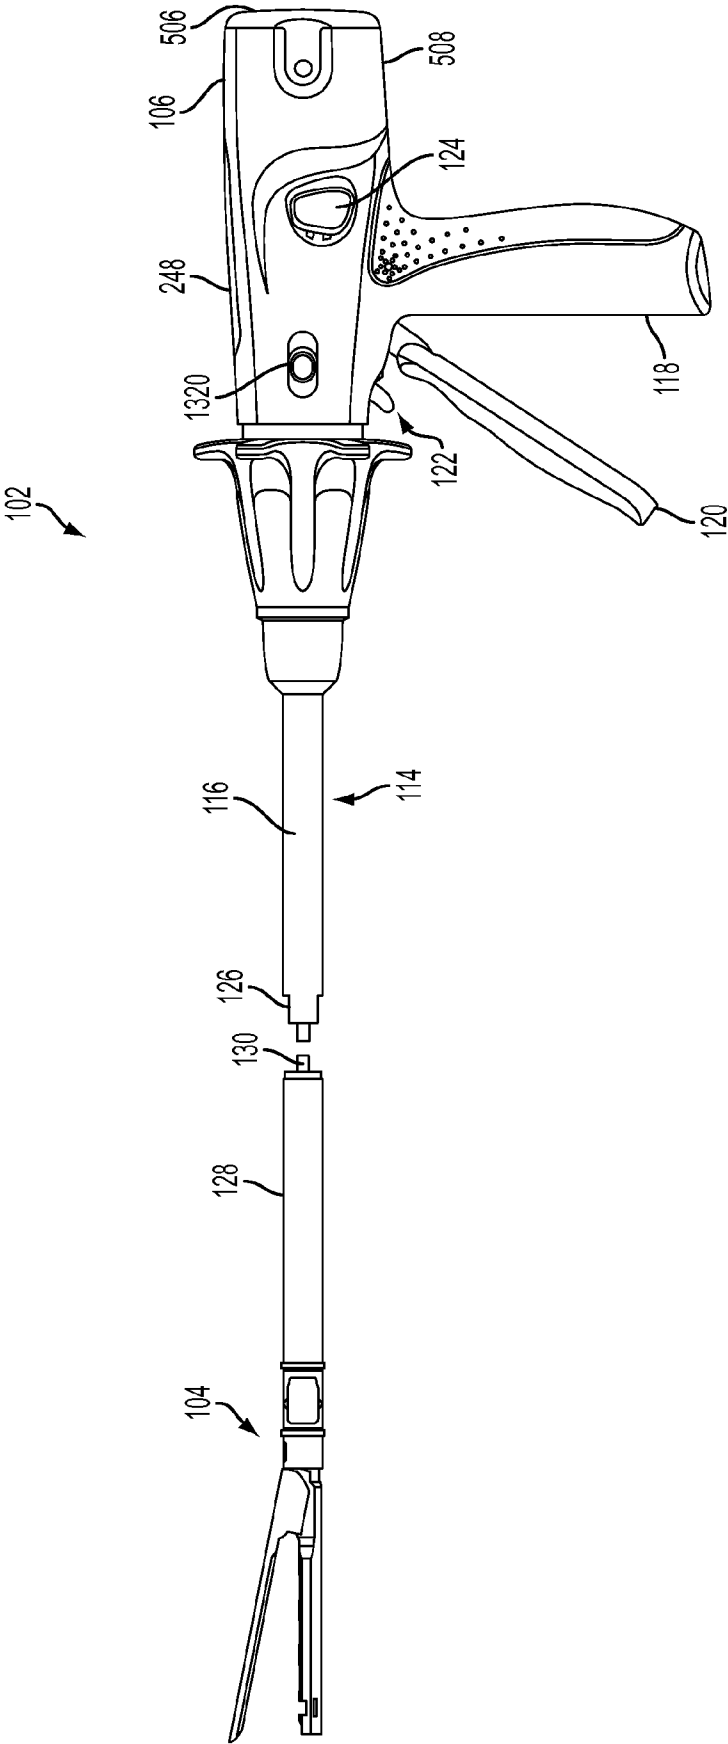


FIG. 1

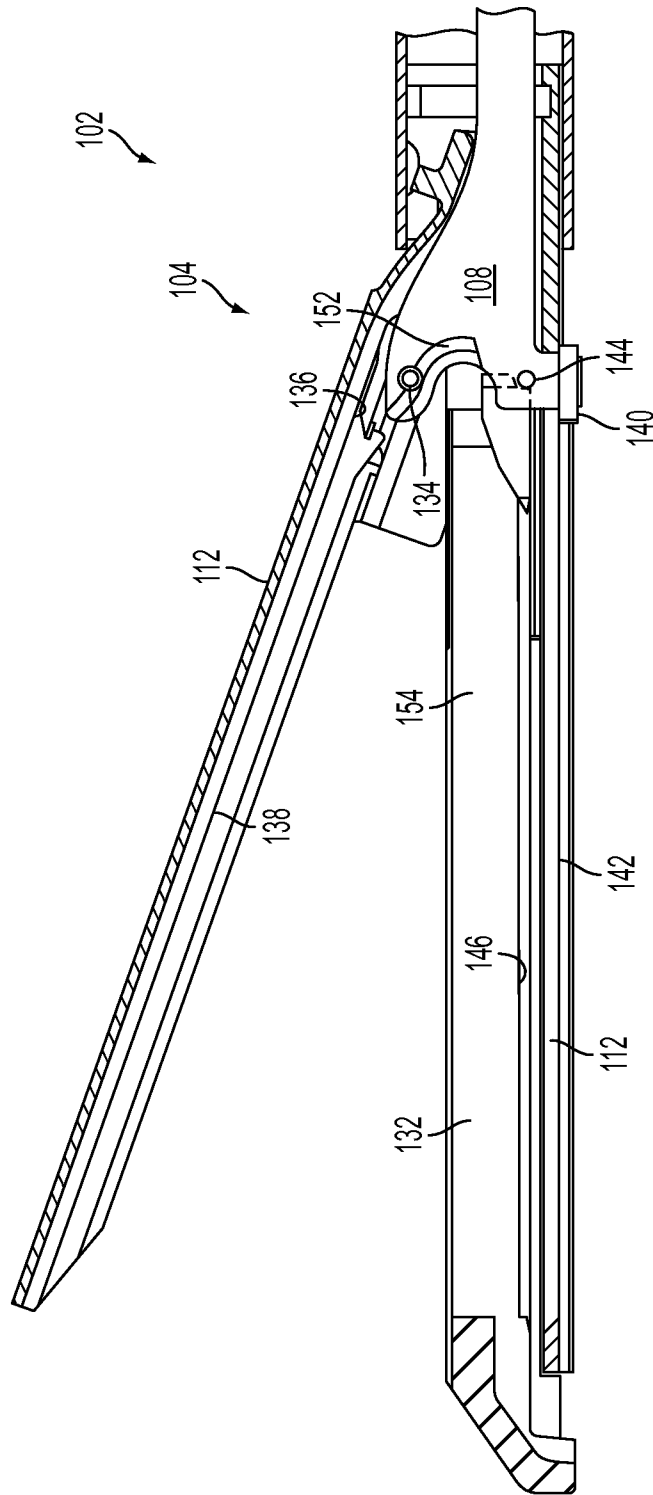


FIG. 2

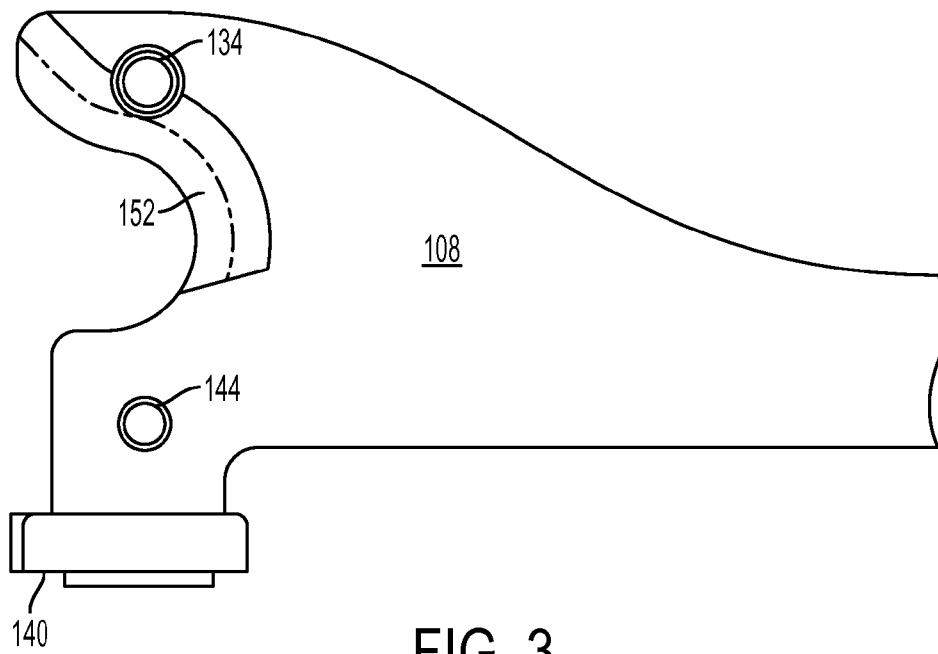


FIG. 3

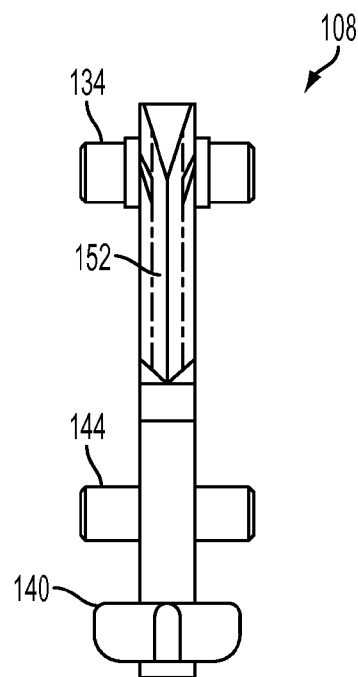


FIG. 4

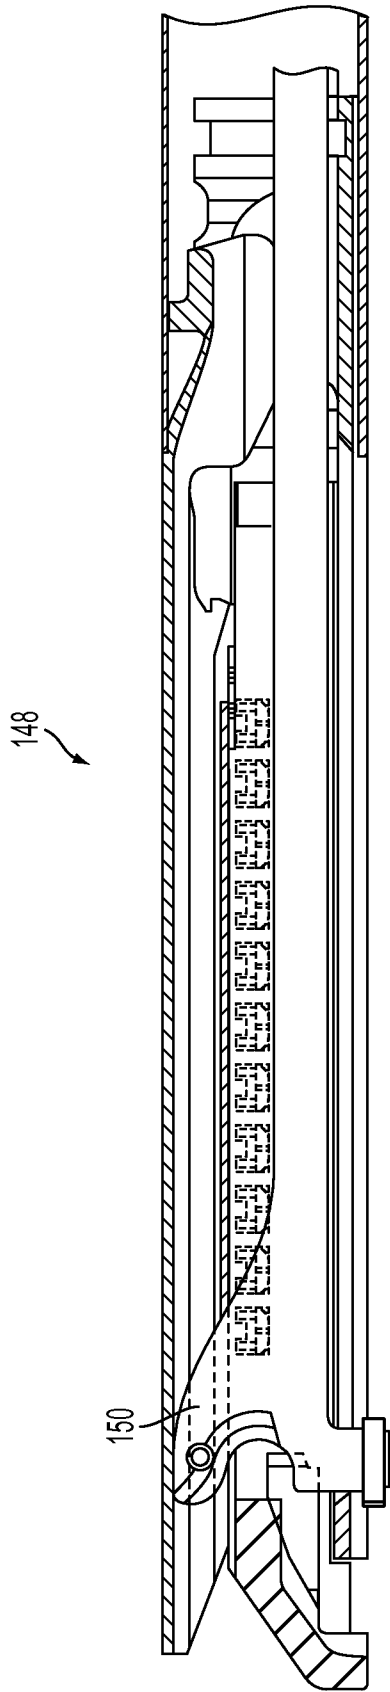


FIG. 5

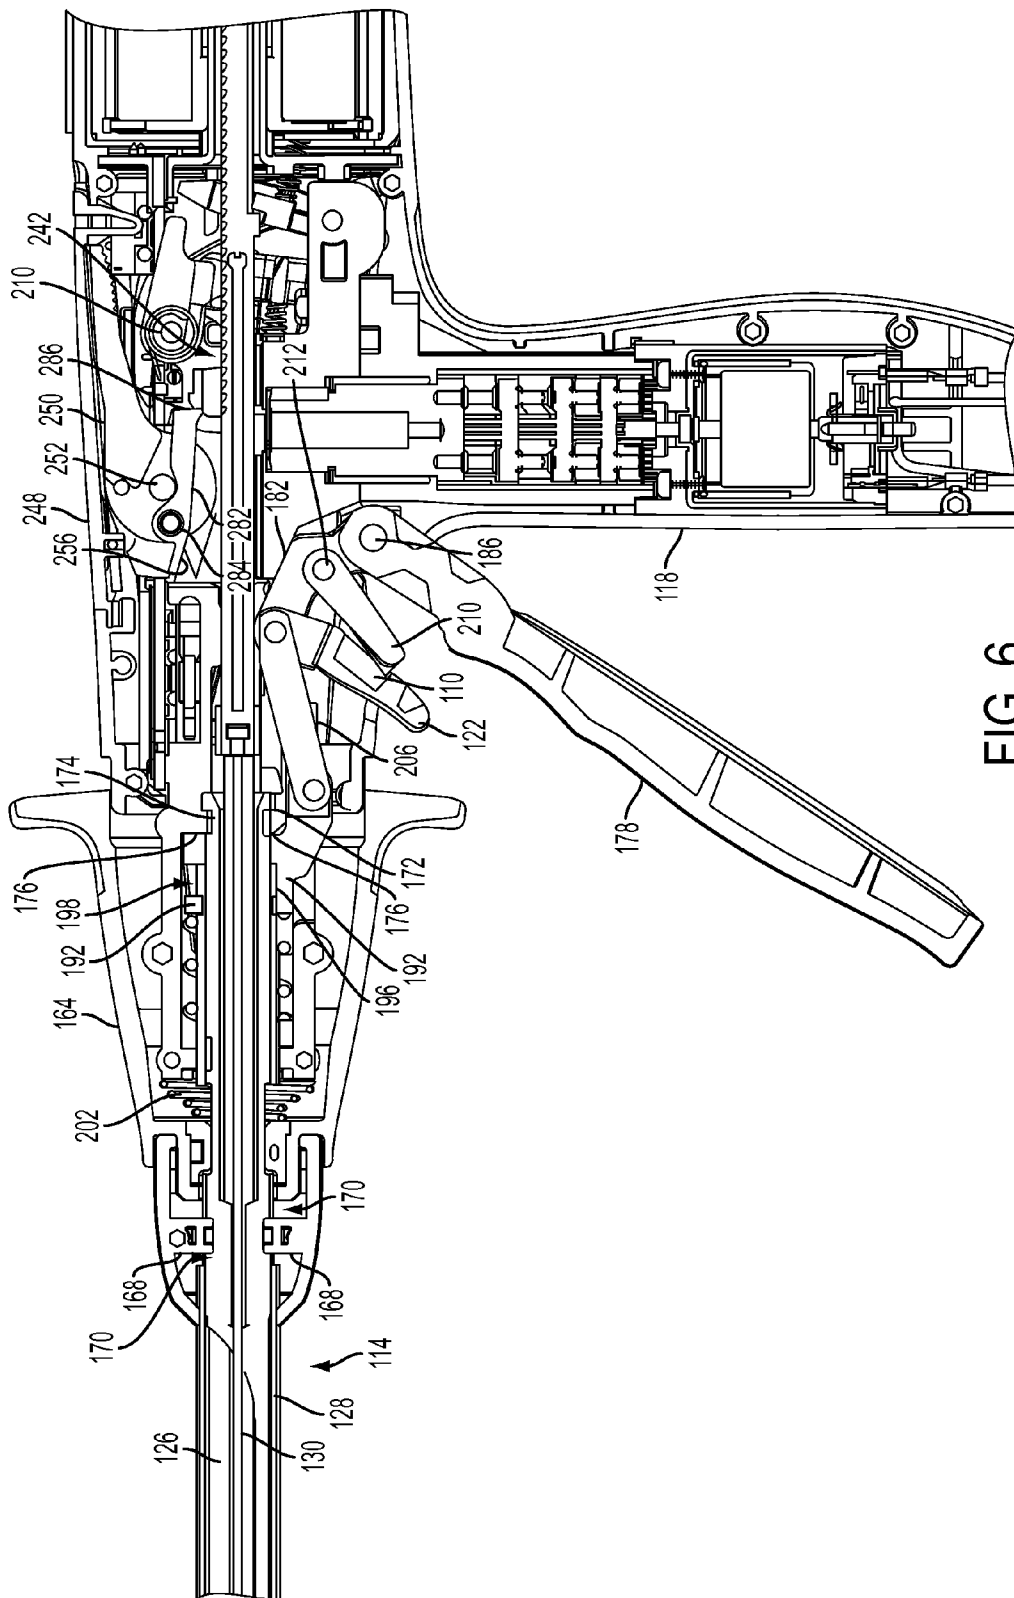
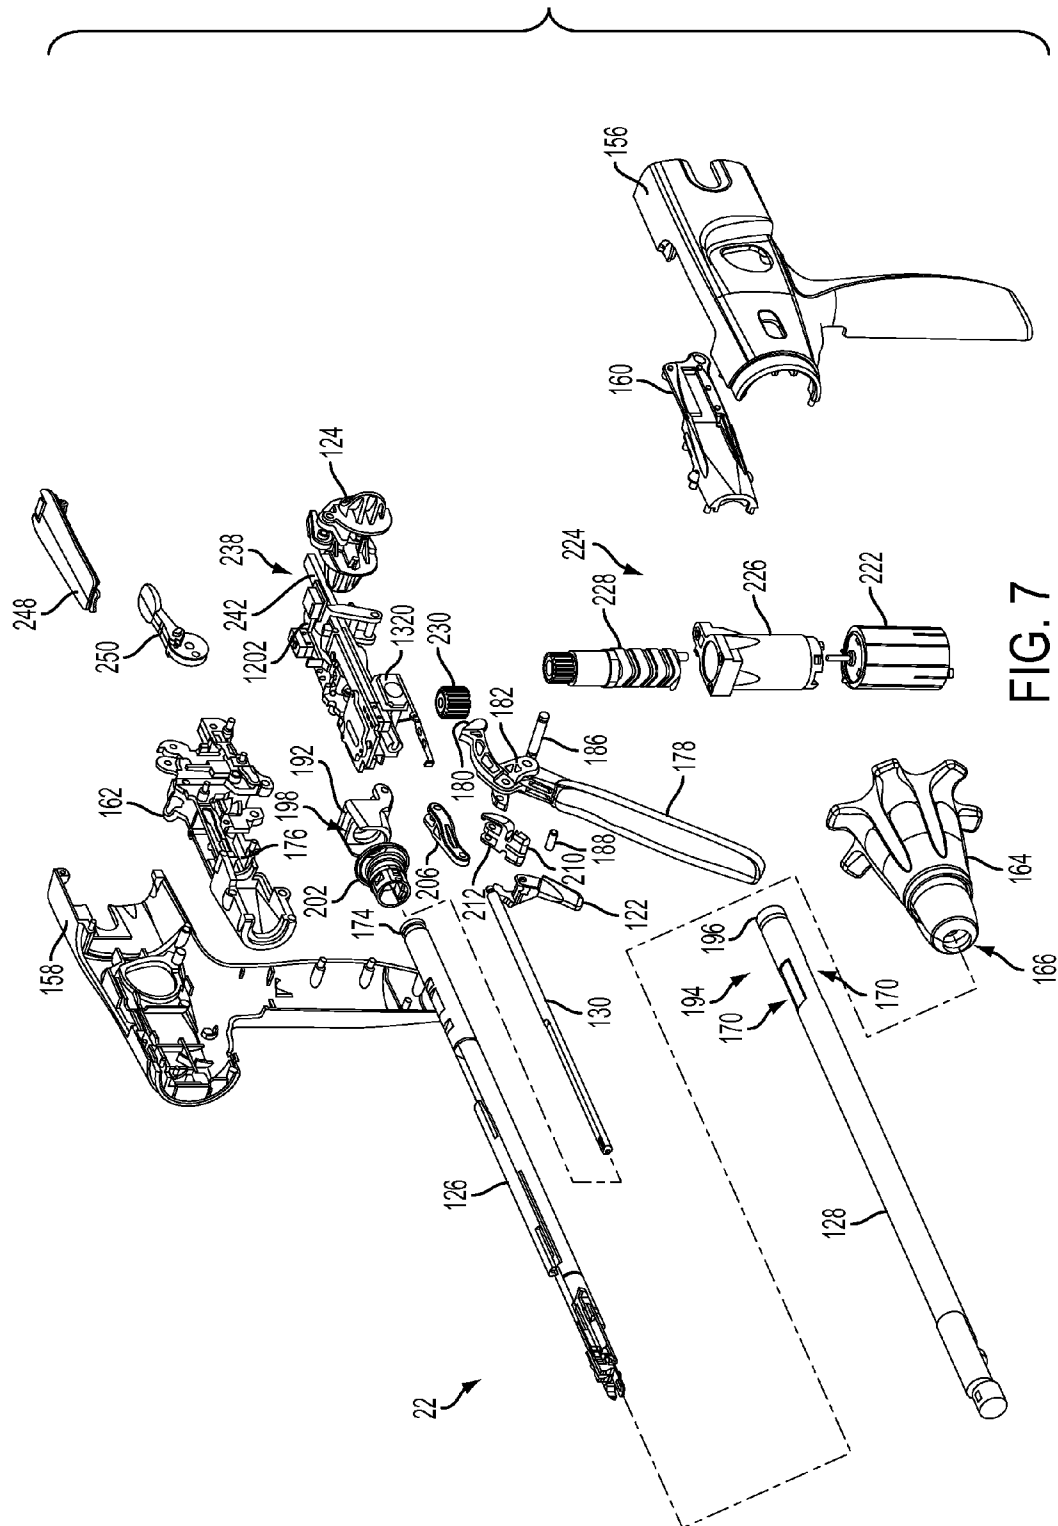


FIG. 6



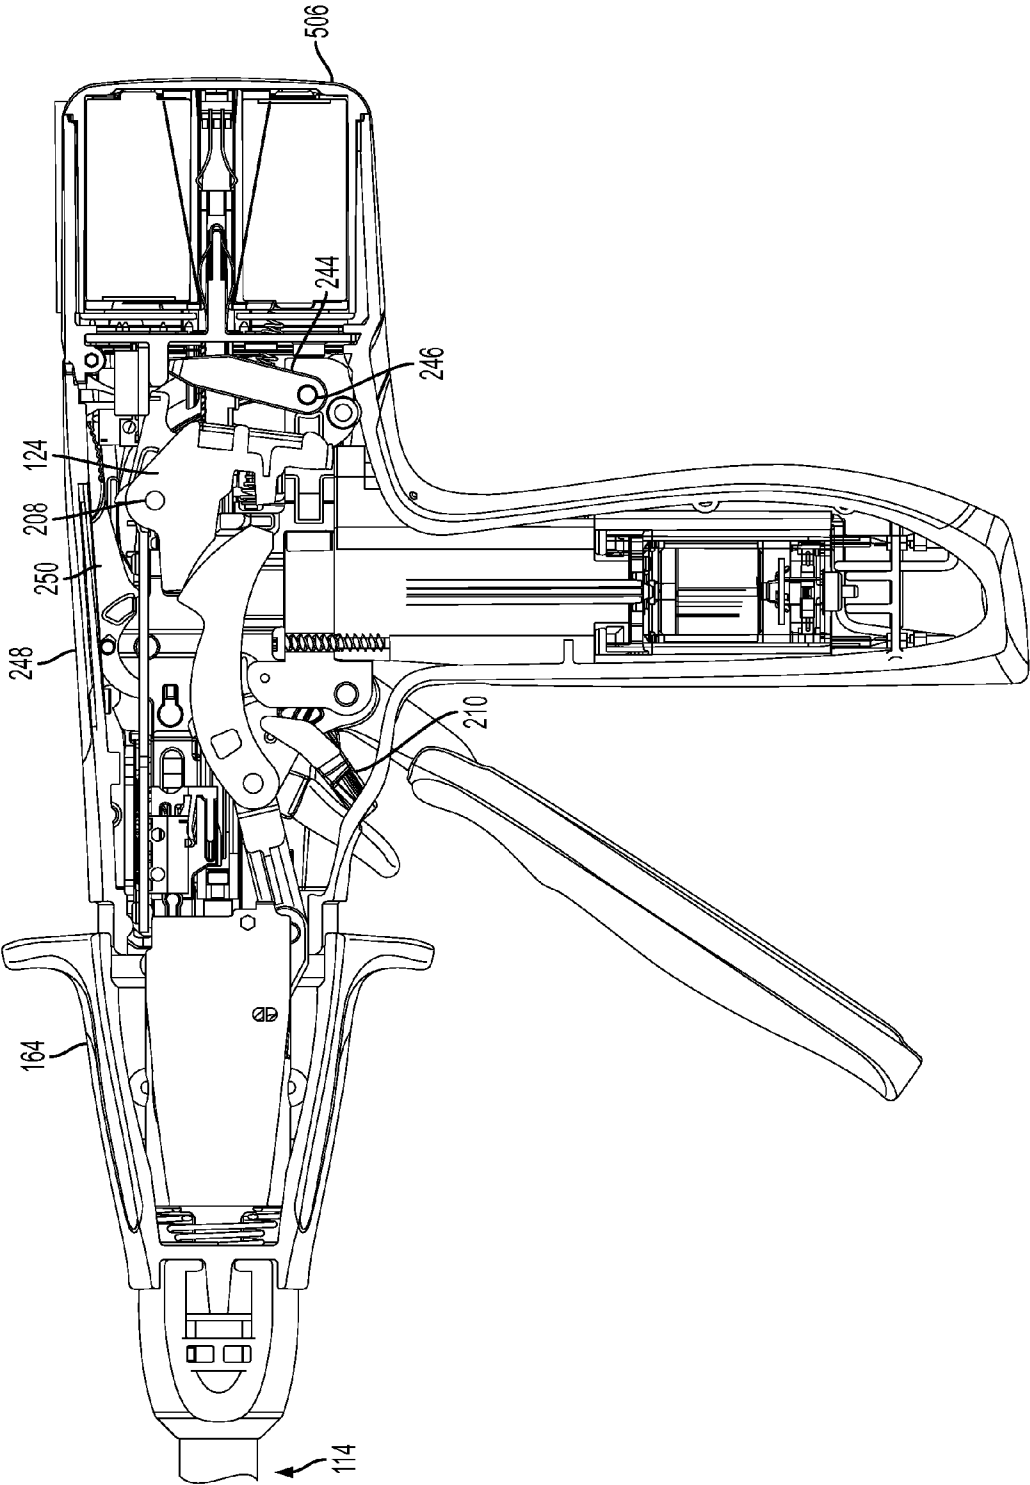


FIG. 8

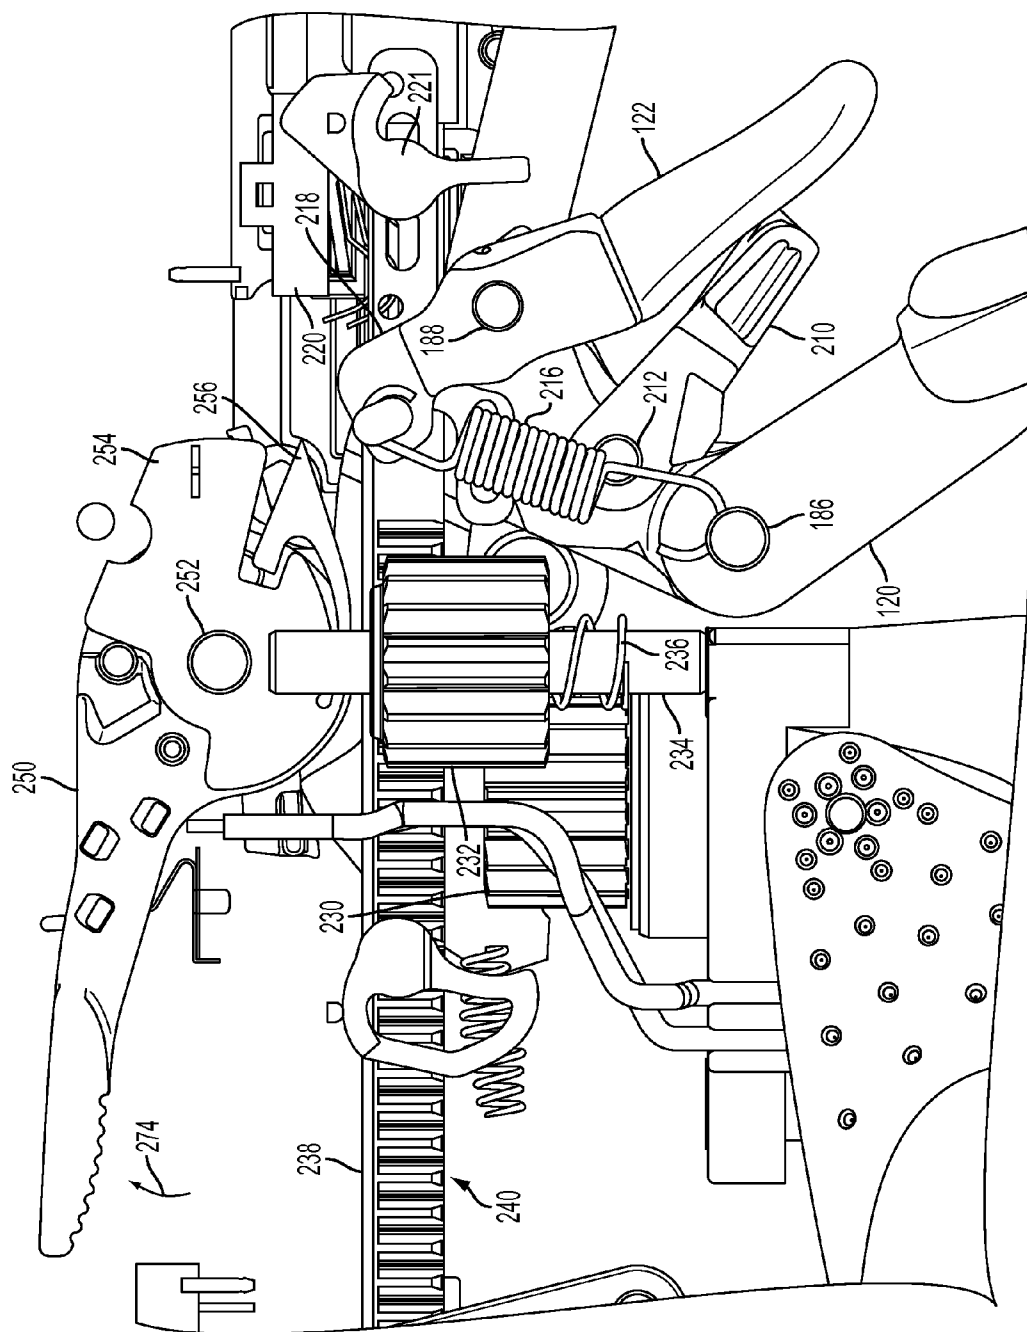


FIG. 9

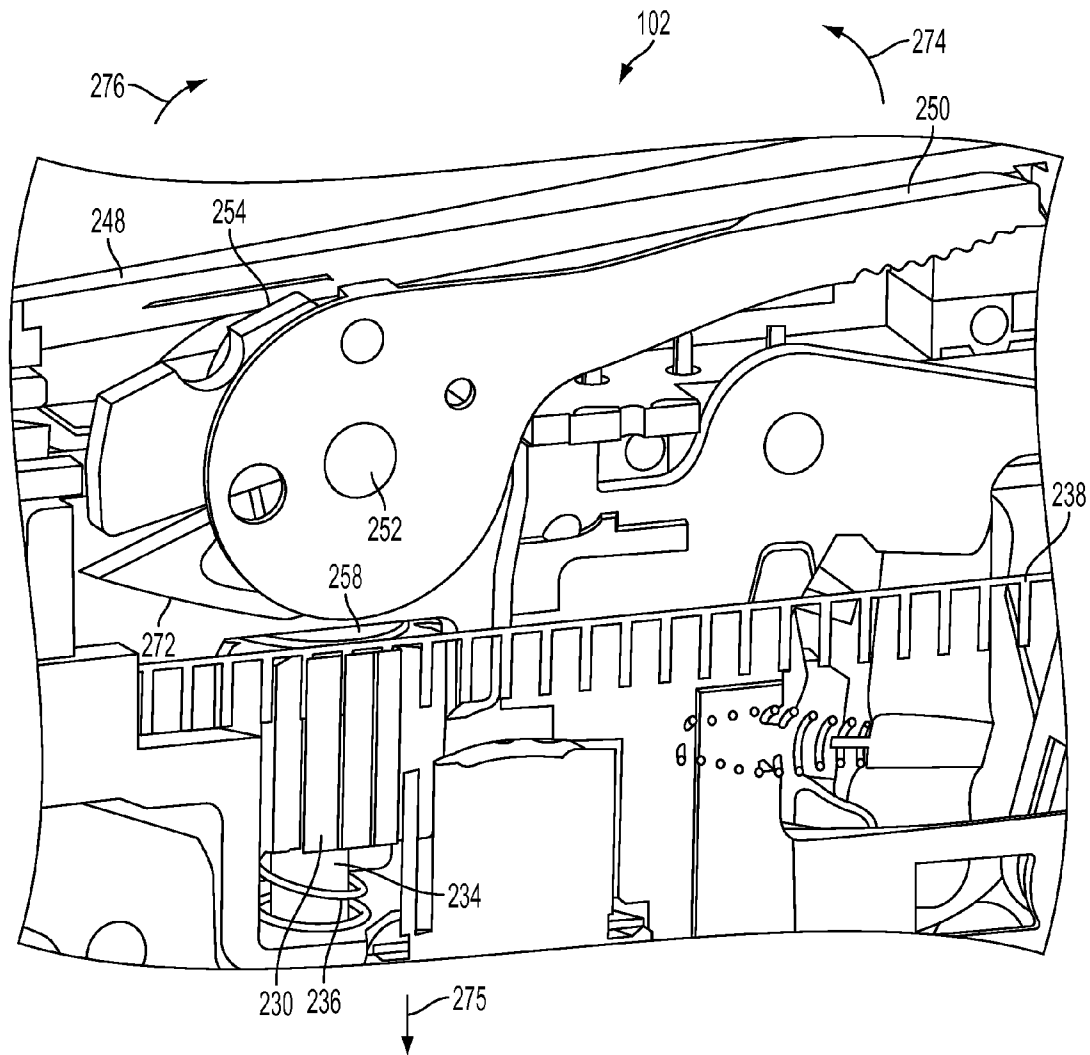


FIG. 10

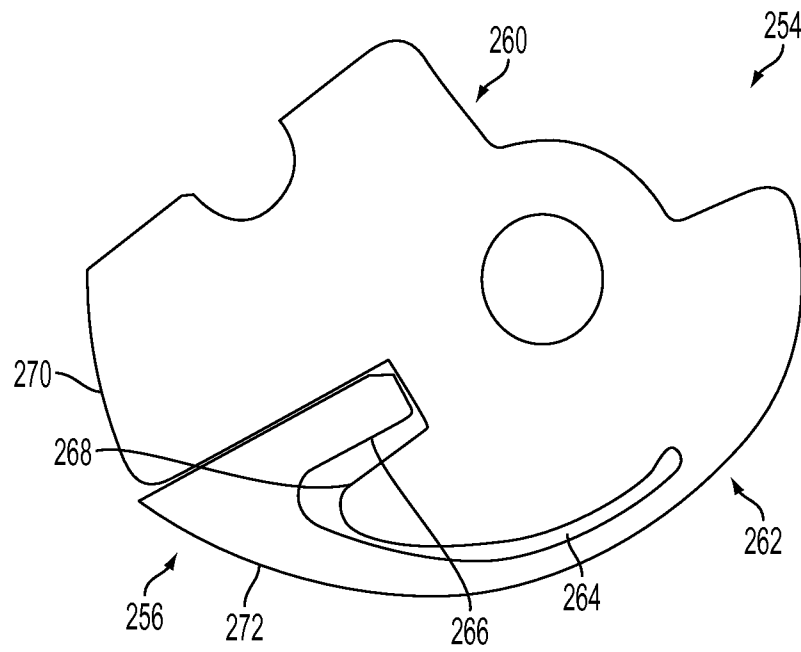


FIG. 11

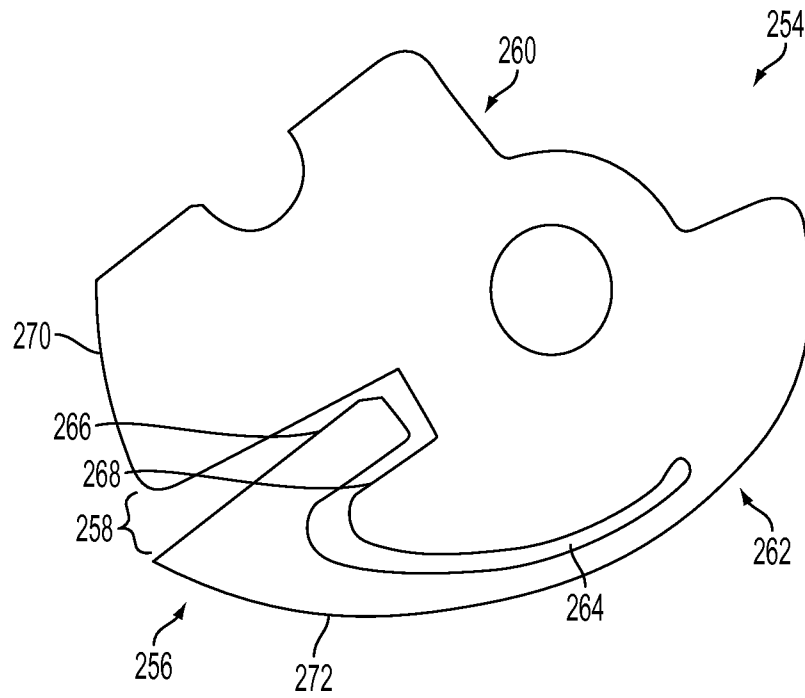


FIG. 12

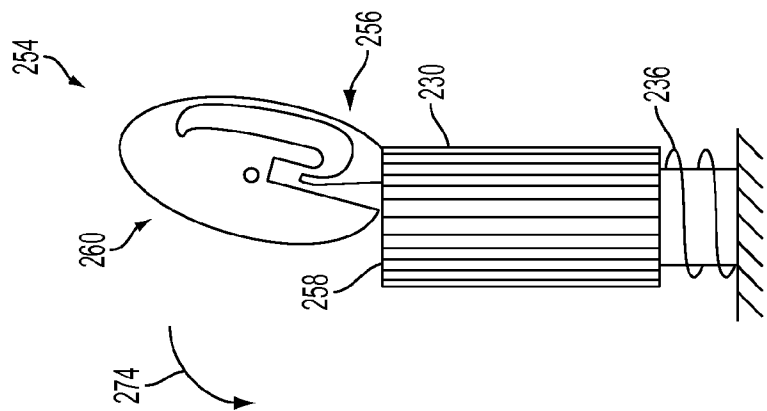


FIG. 13

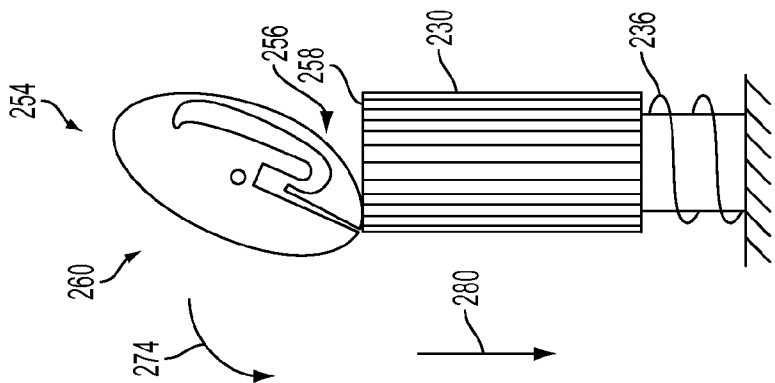


FIG. 14

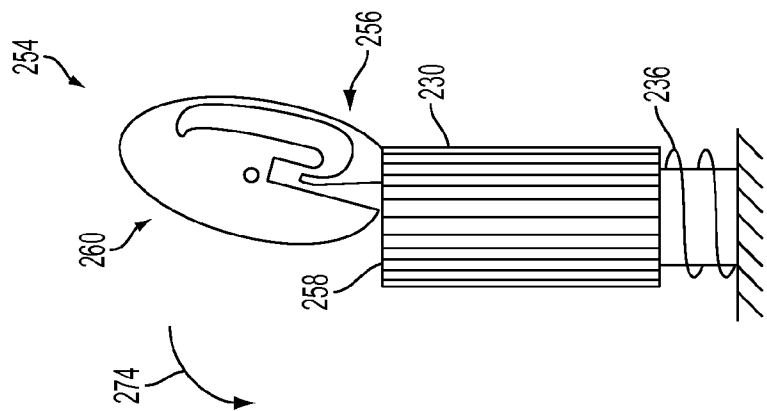


FIG. 15

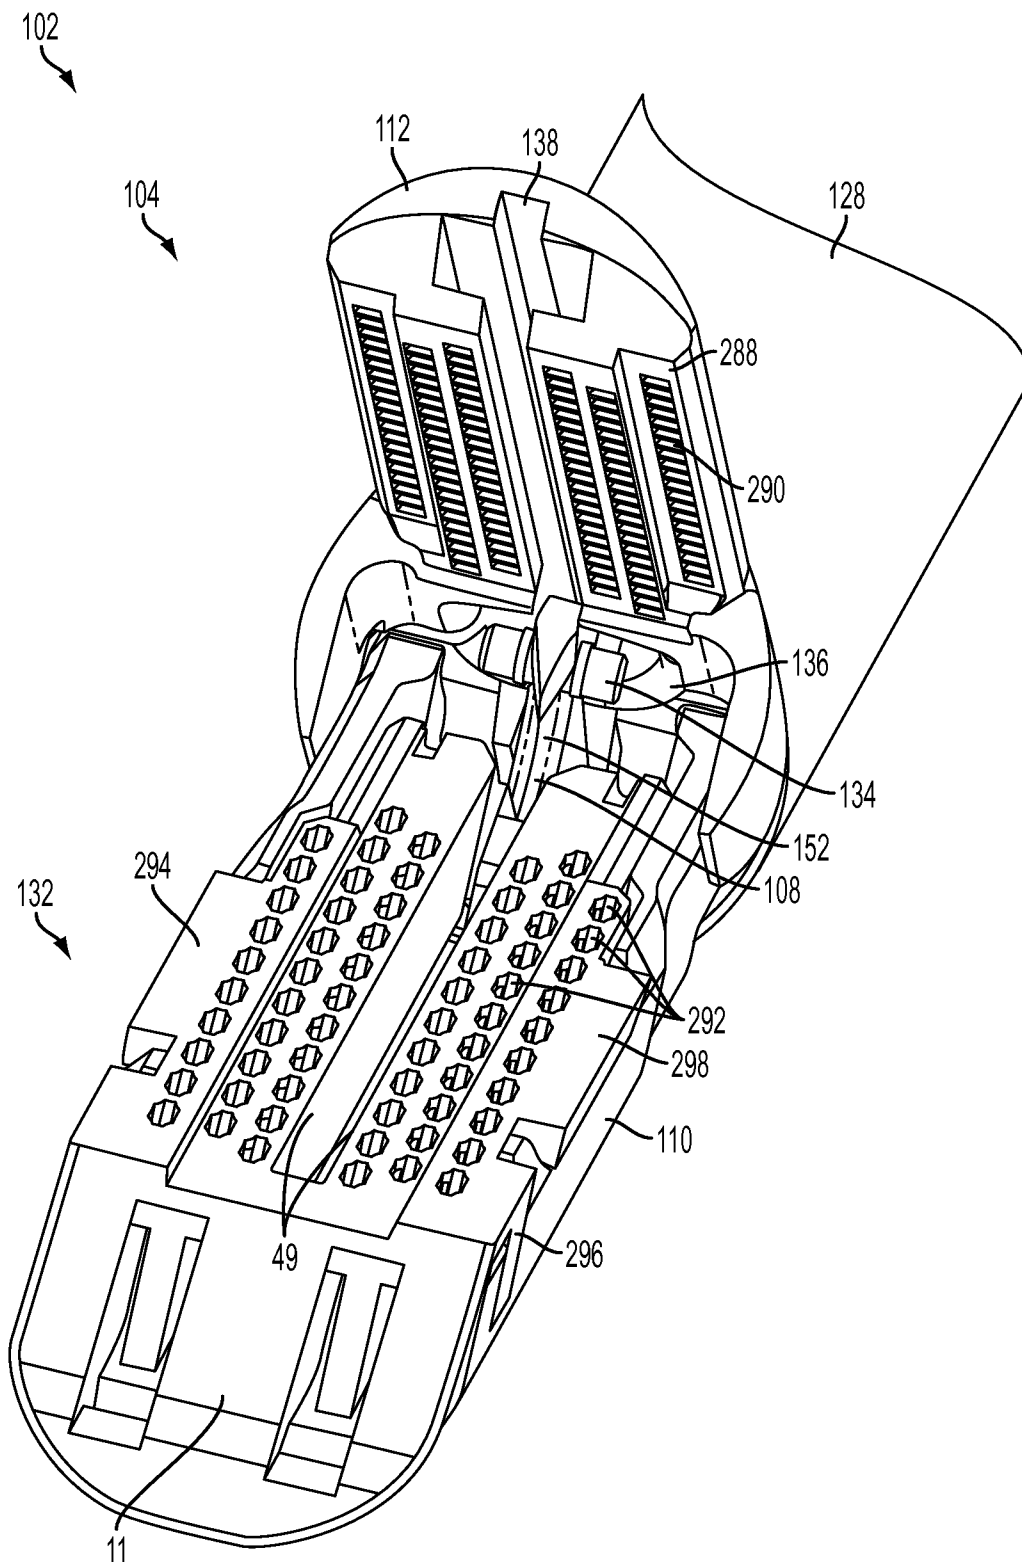


FIG. 16

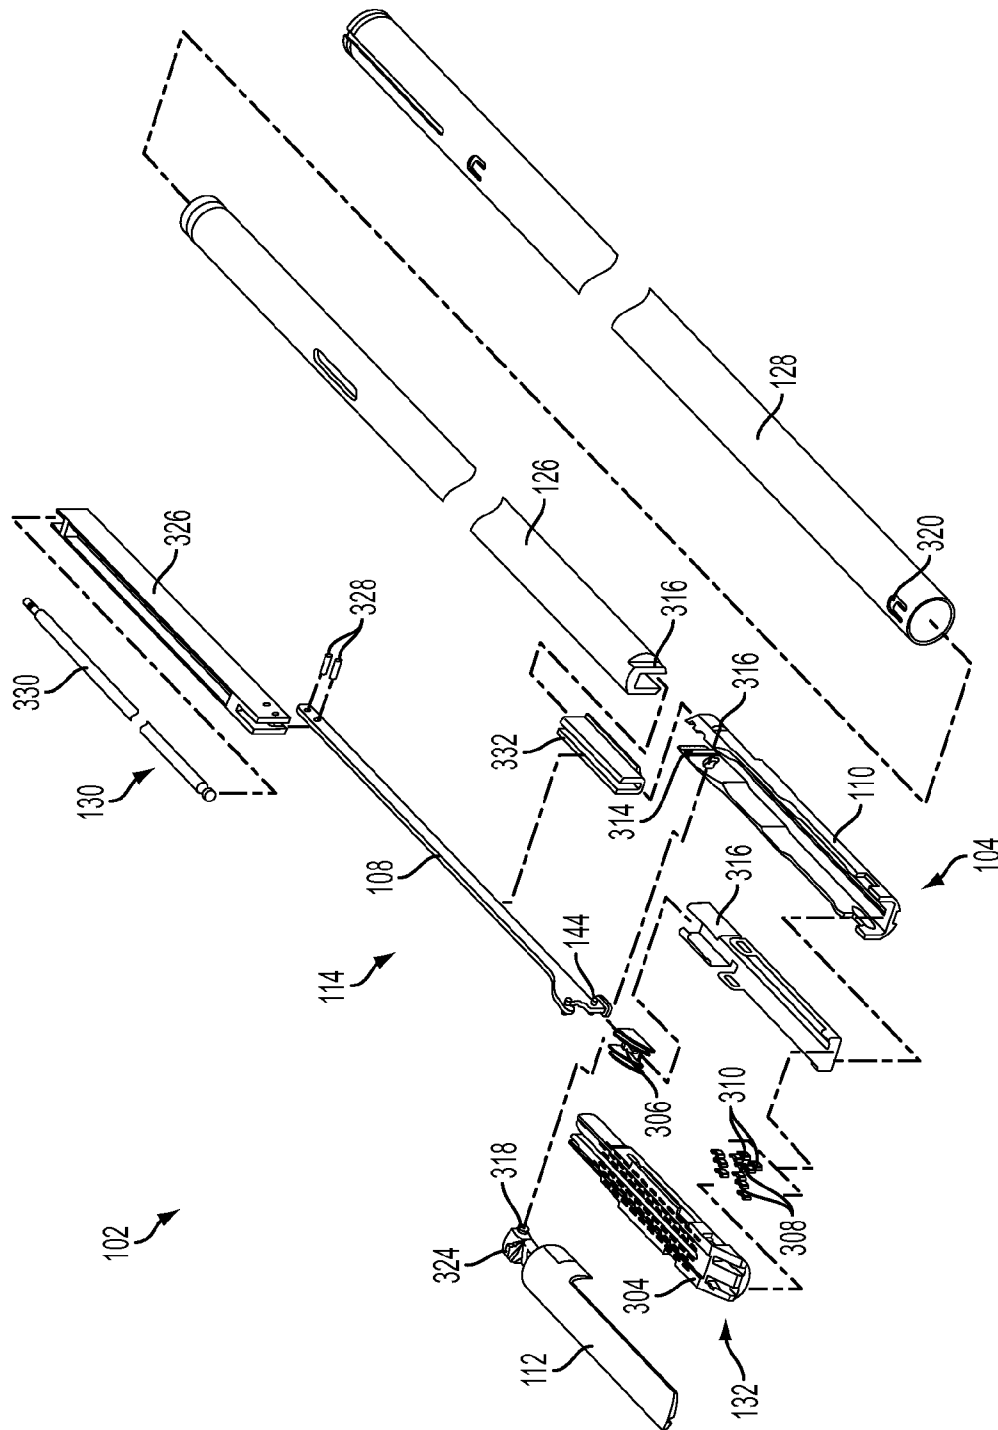


FIG. 17

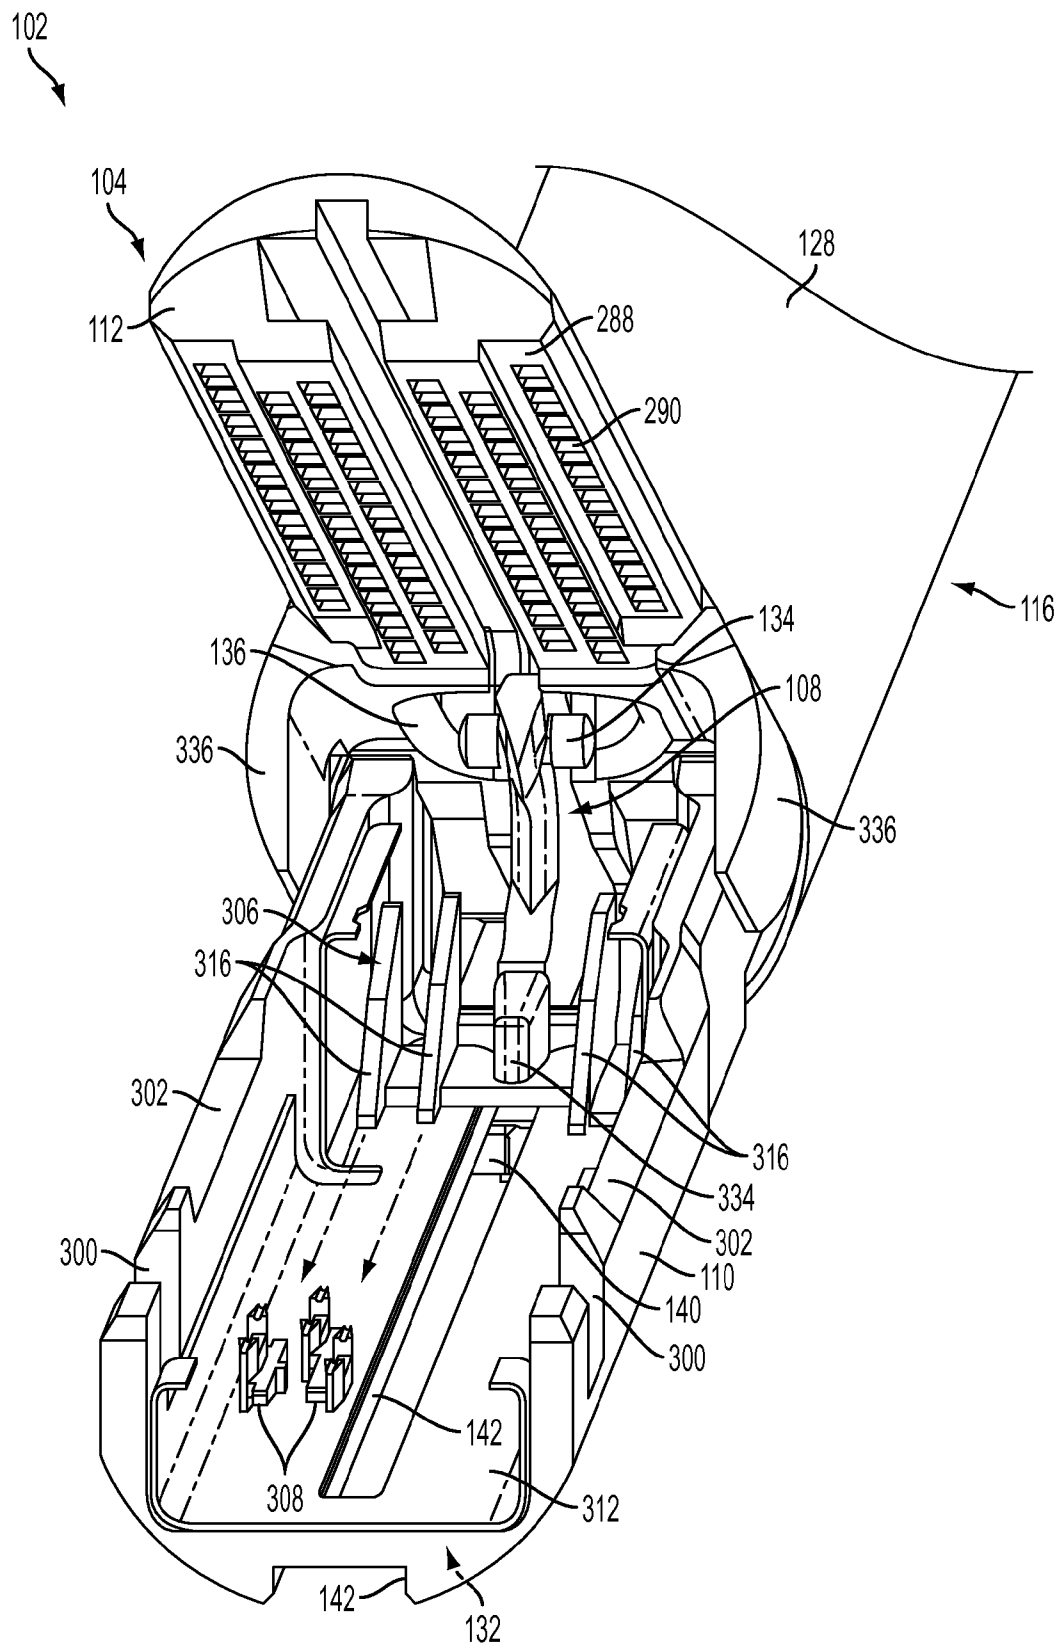


FIG. 18

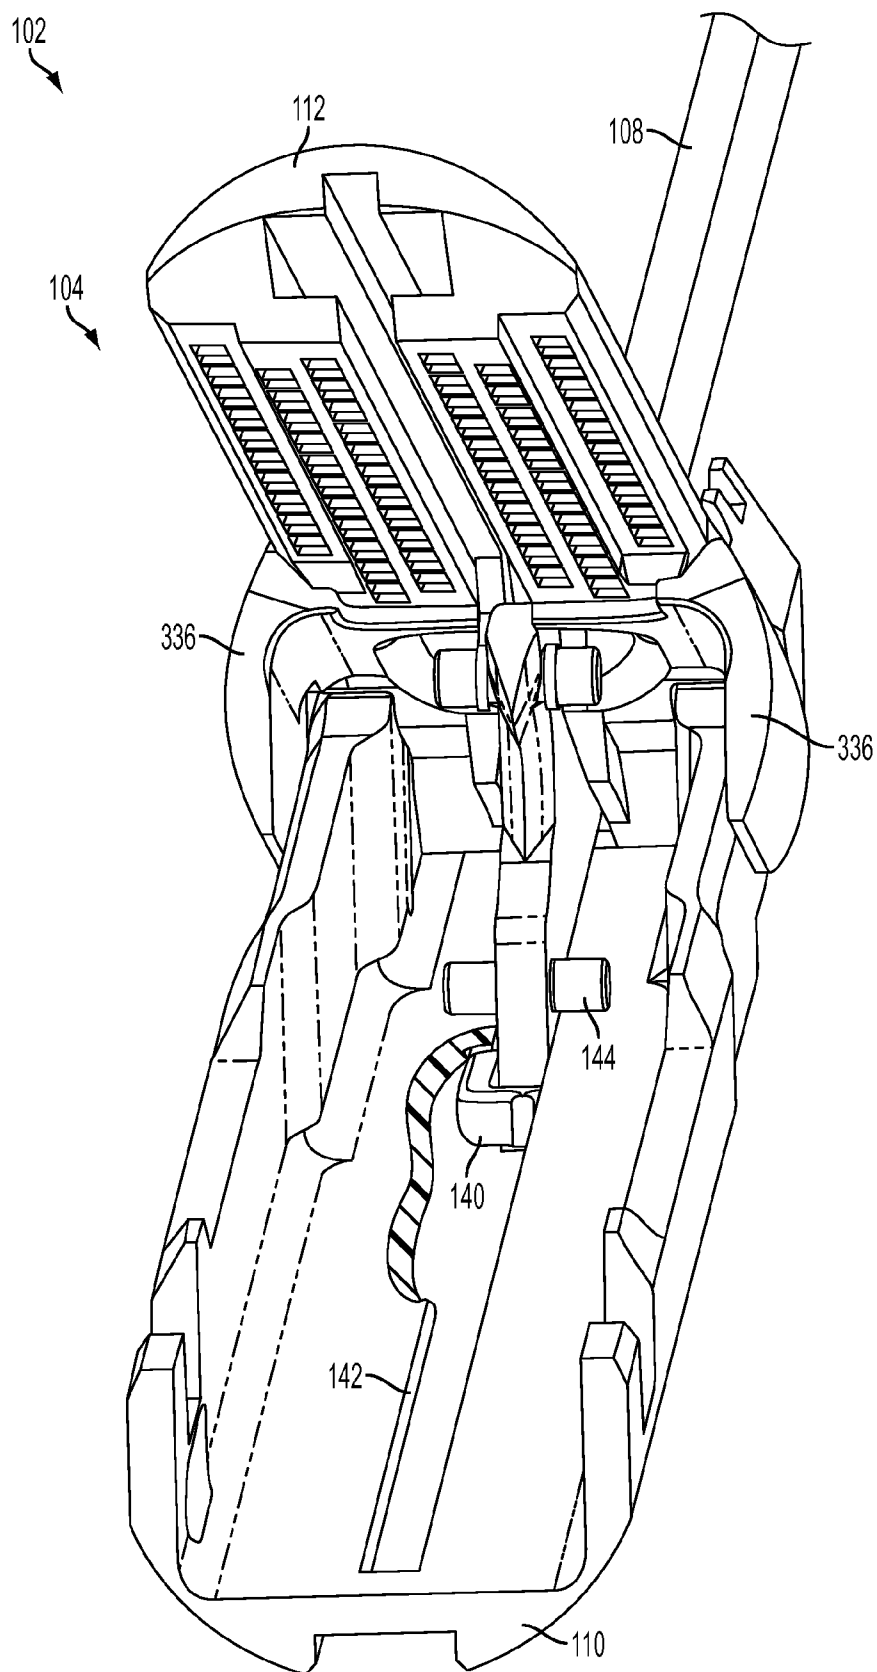


FIG. 19

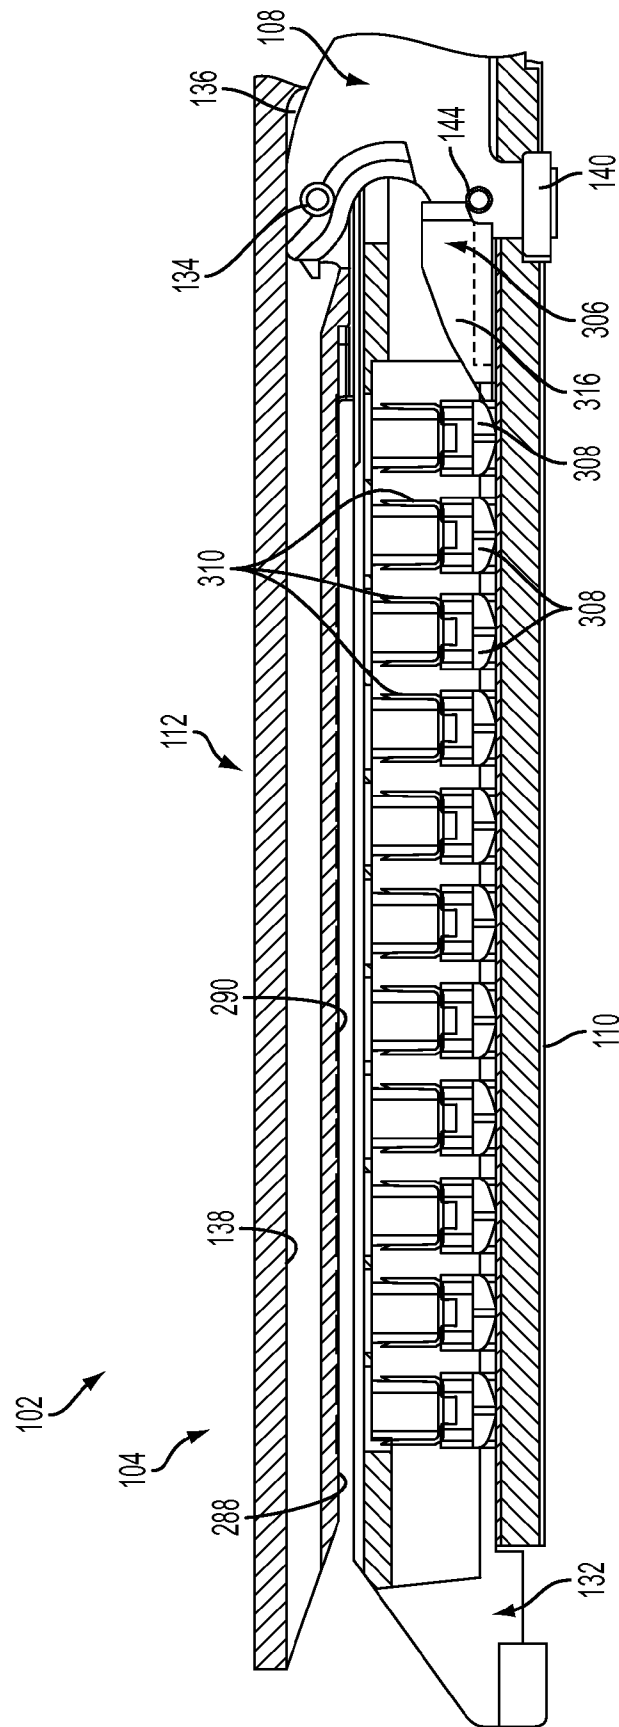


FIG. 20

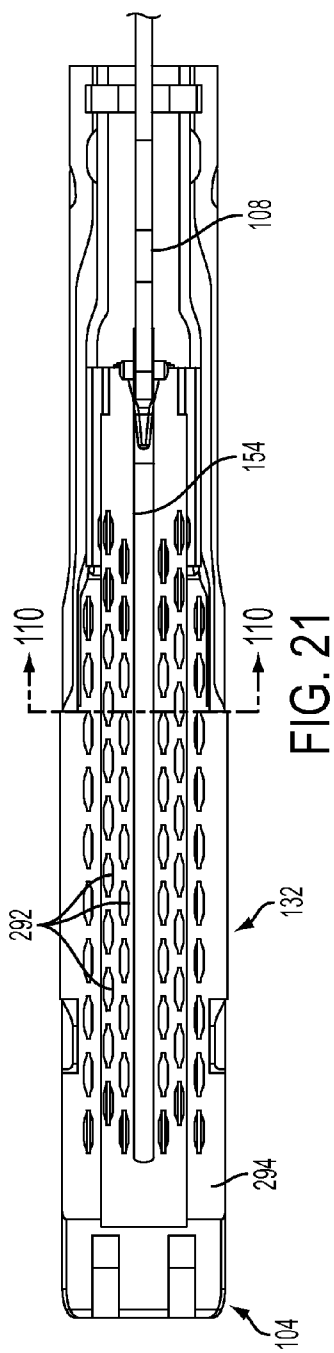


FIG. 21

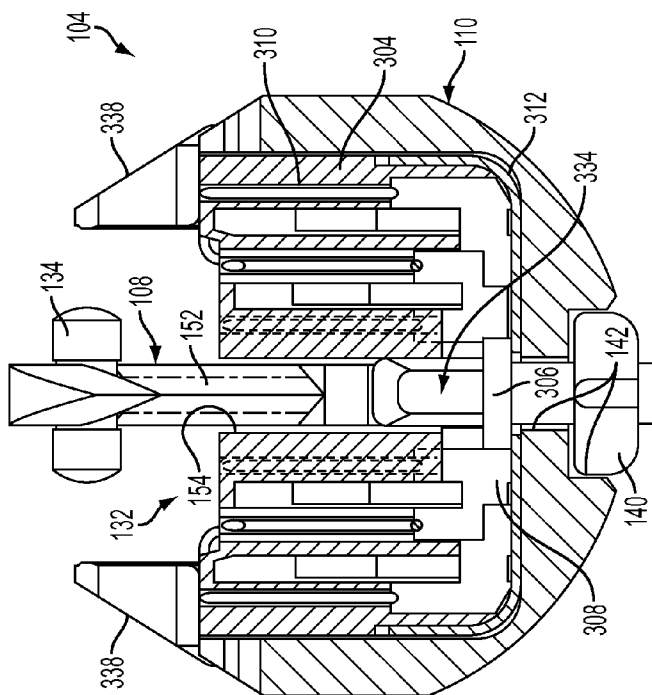


FIG. 22

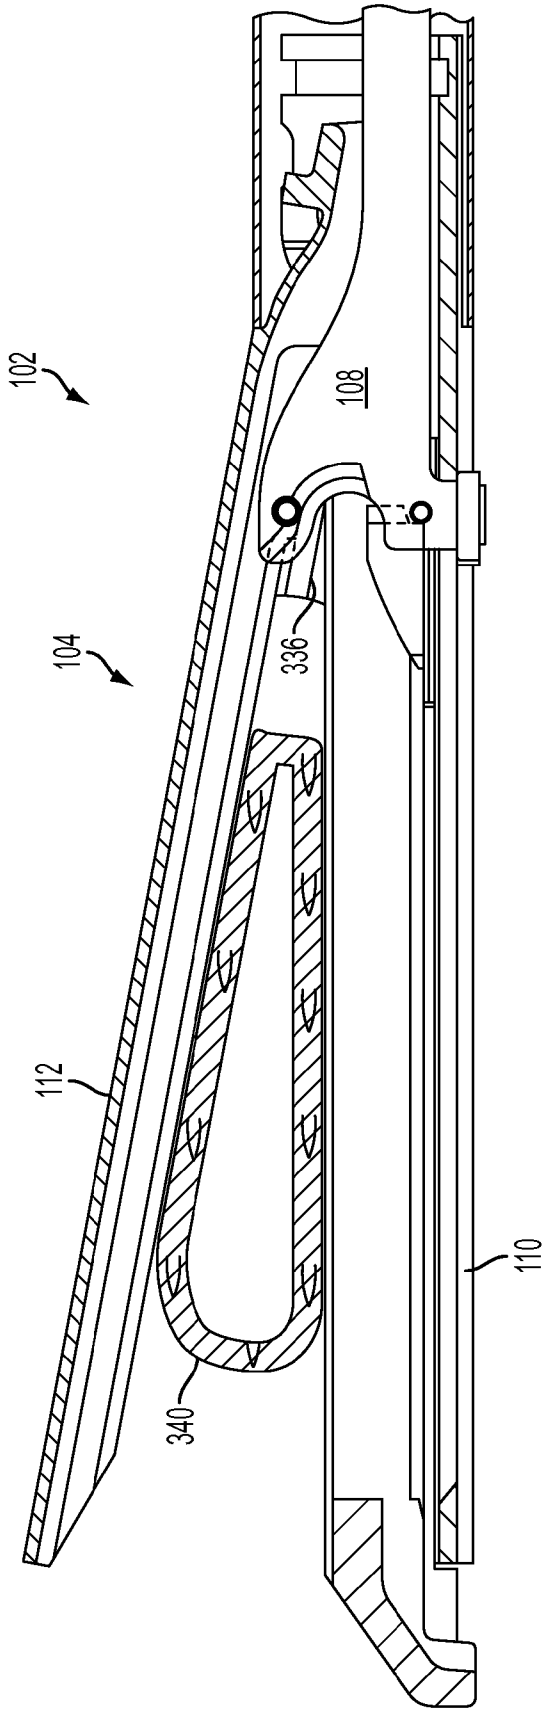


FIG. 23

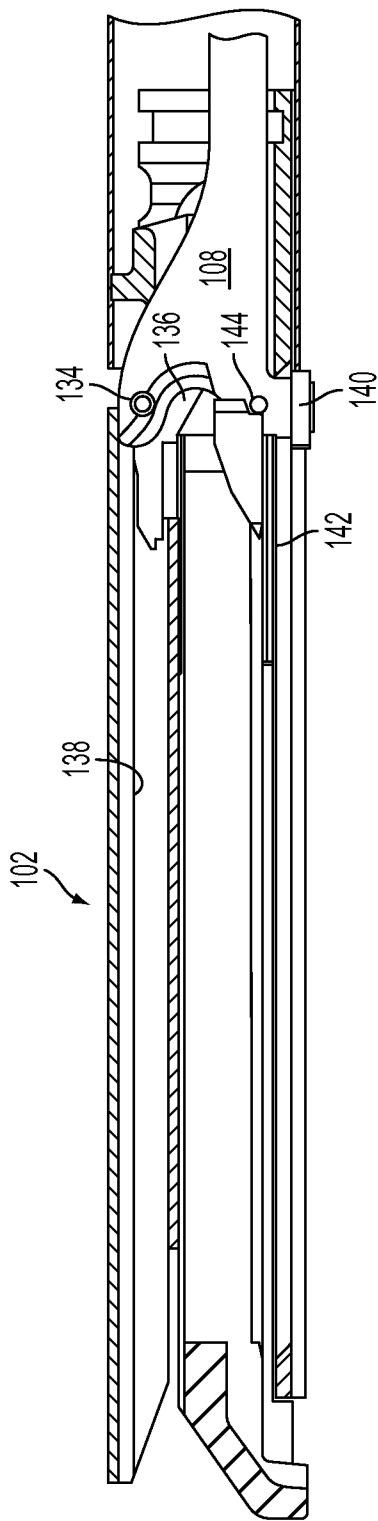


FIG. 24

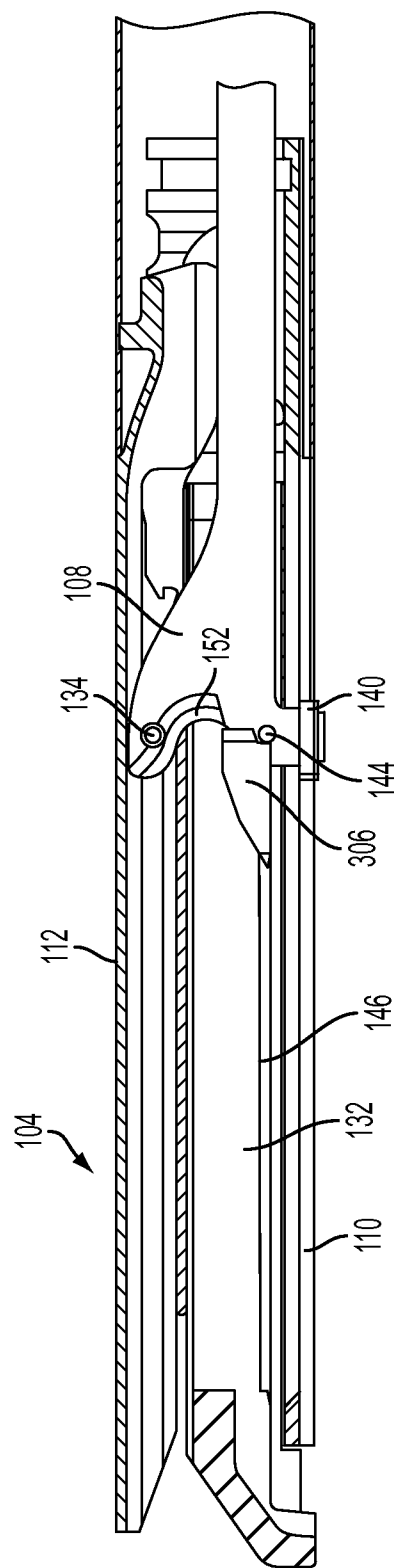


FIG. 25

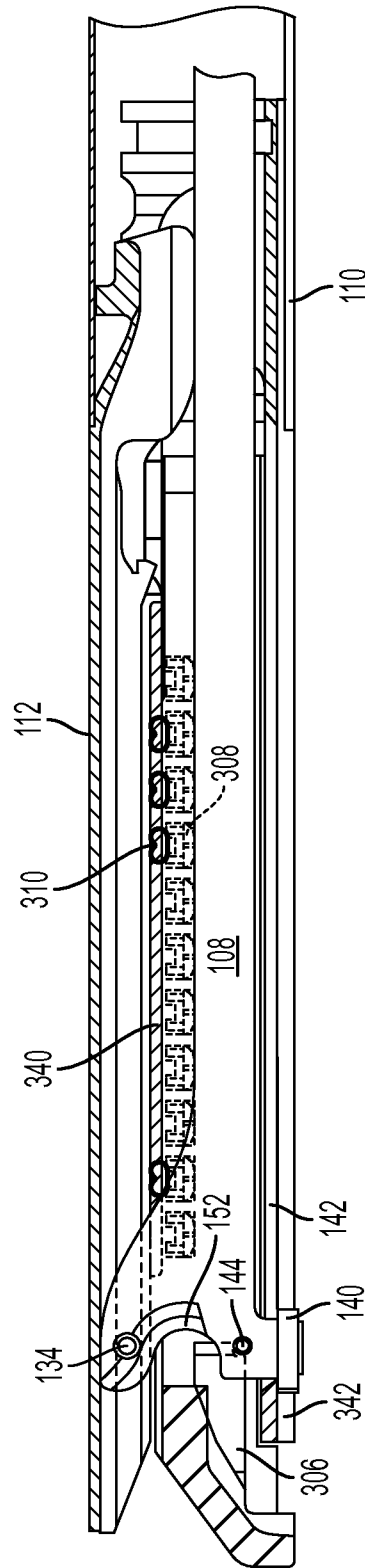


FIG. 26

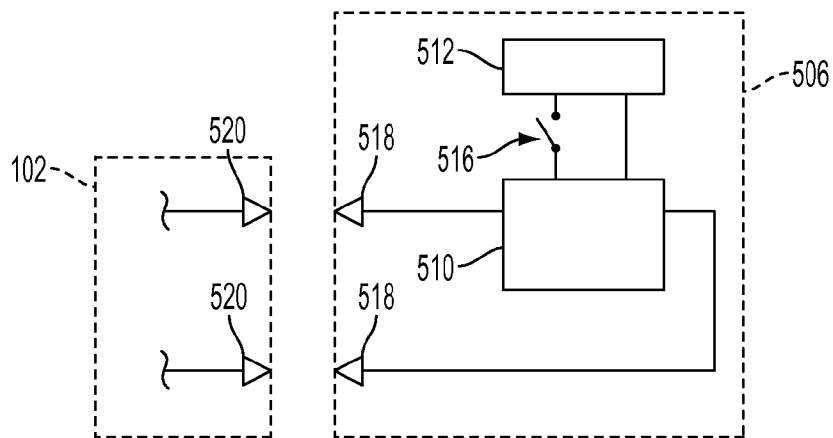


FIG. 27

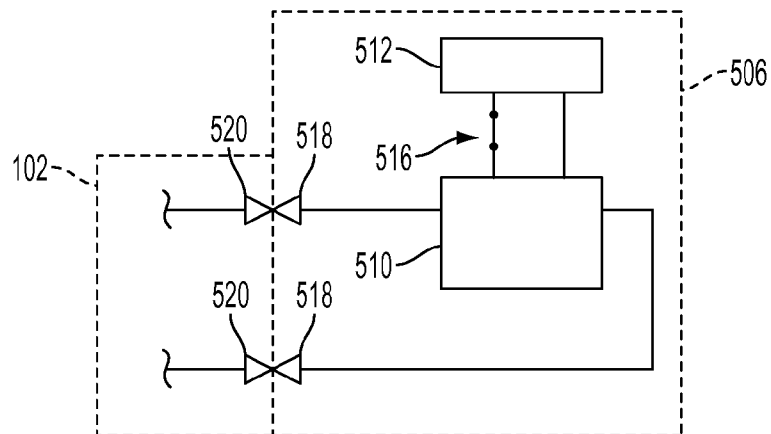


FIG. 28

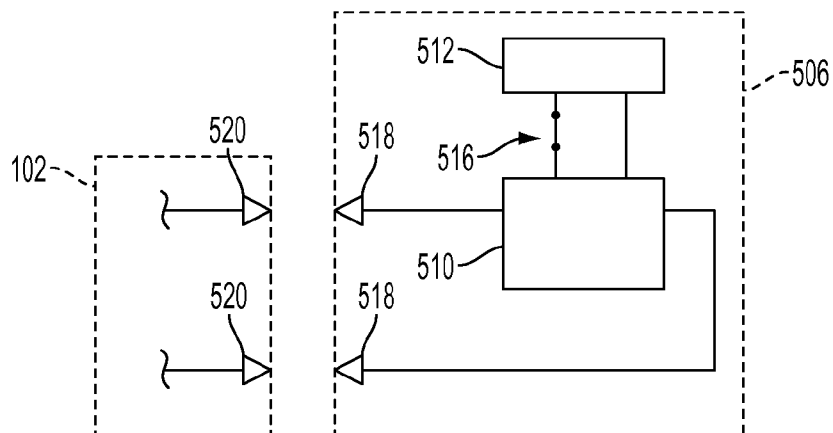


FIG. 29

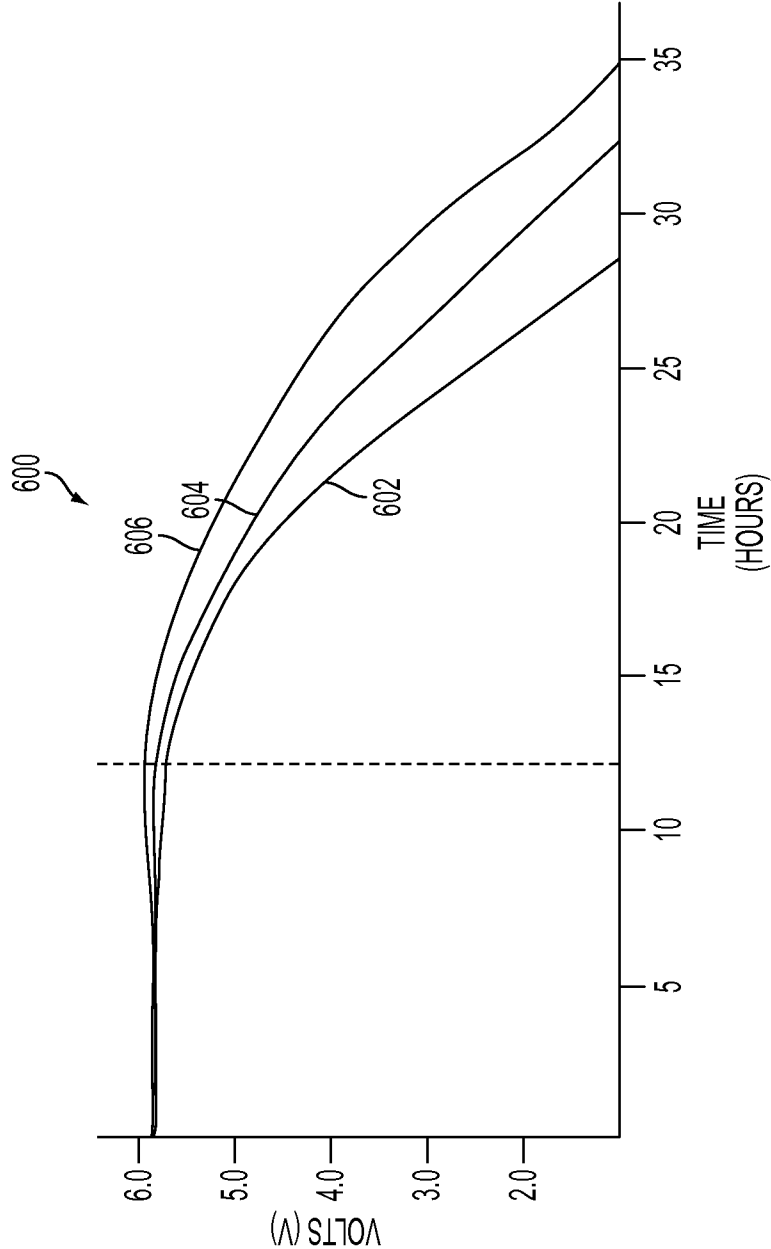


FIG. 30

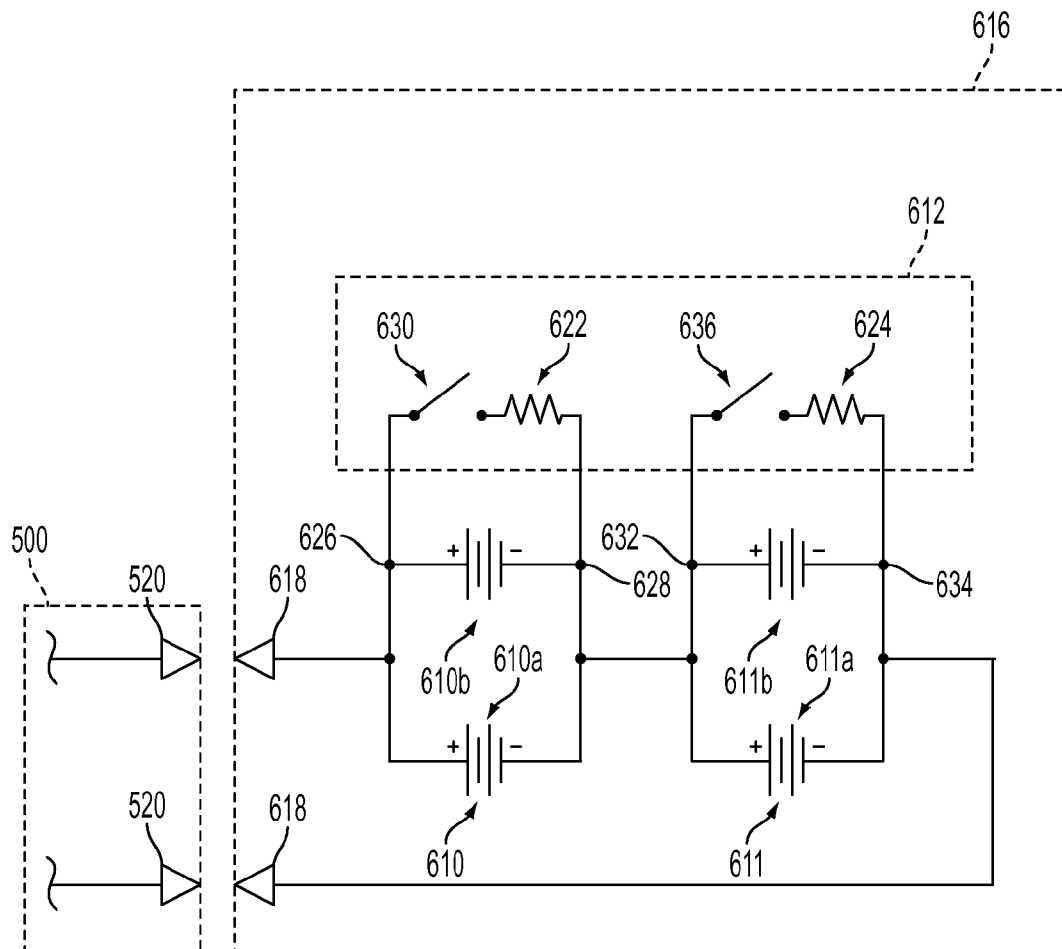


FIG. 31

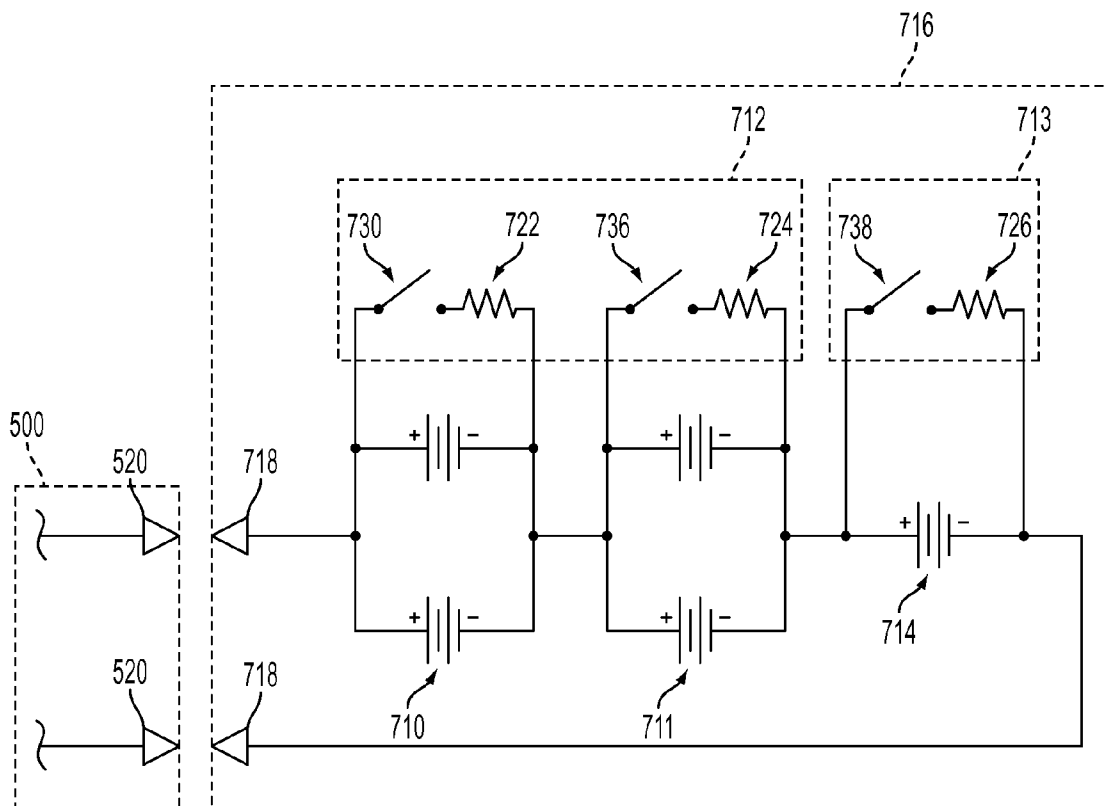


FIG. 32

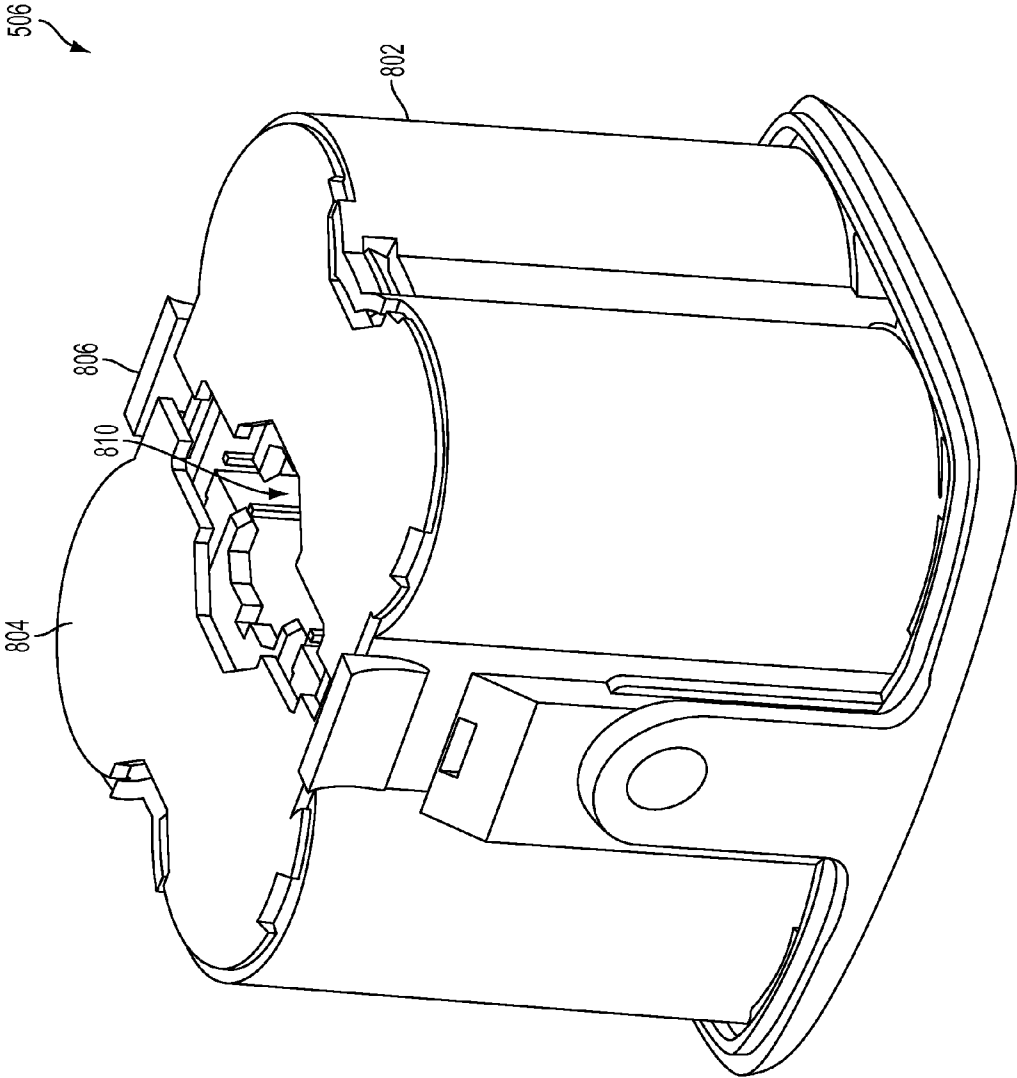


FIG. 33

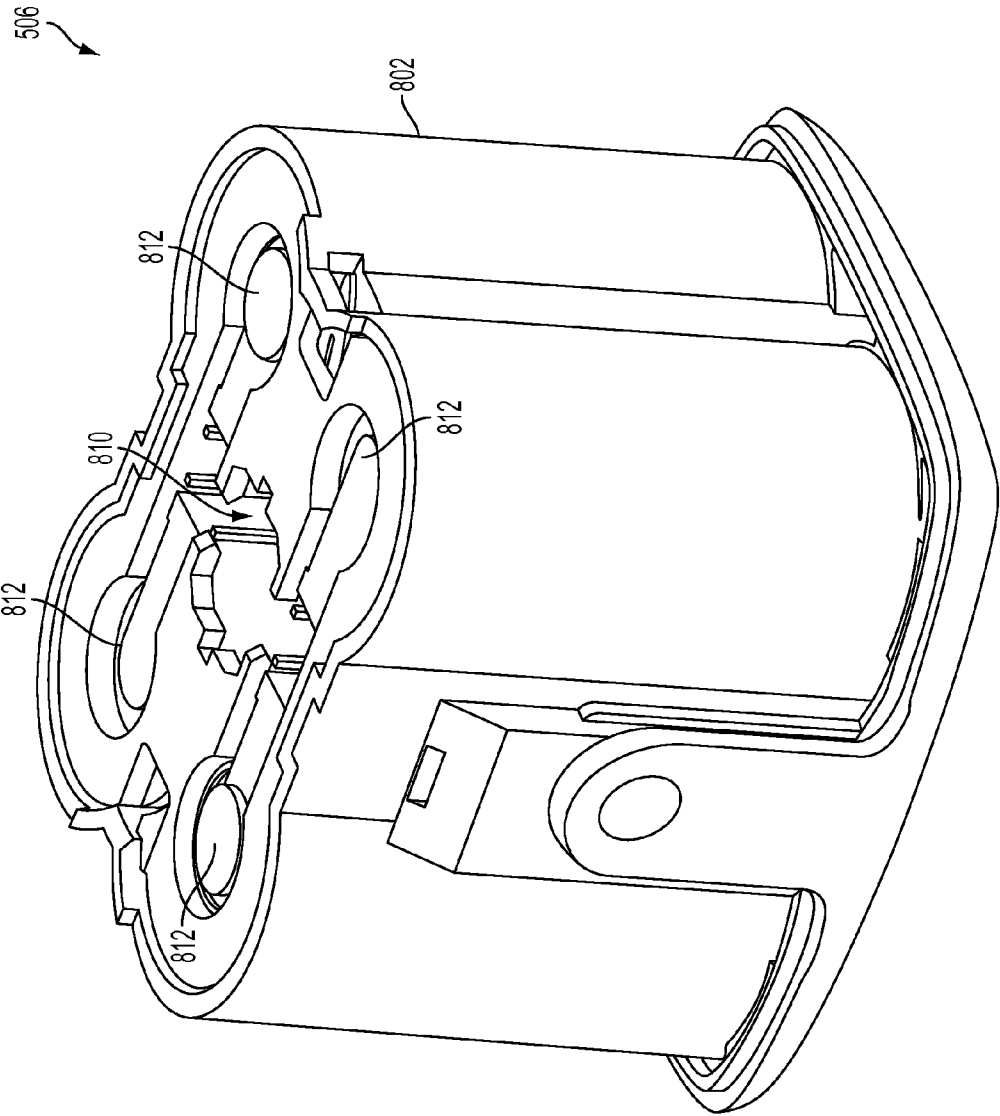


FIG. 34

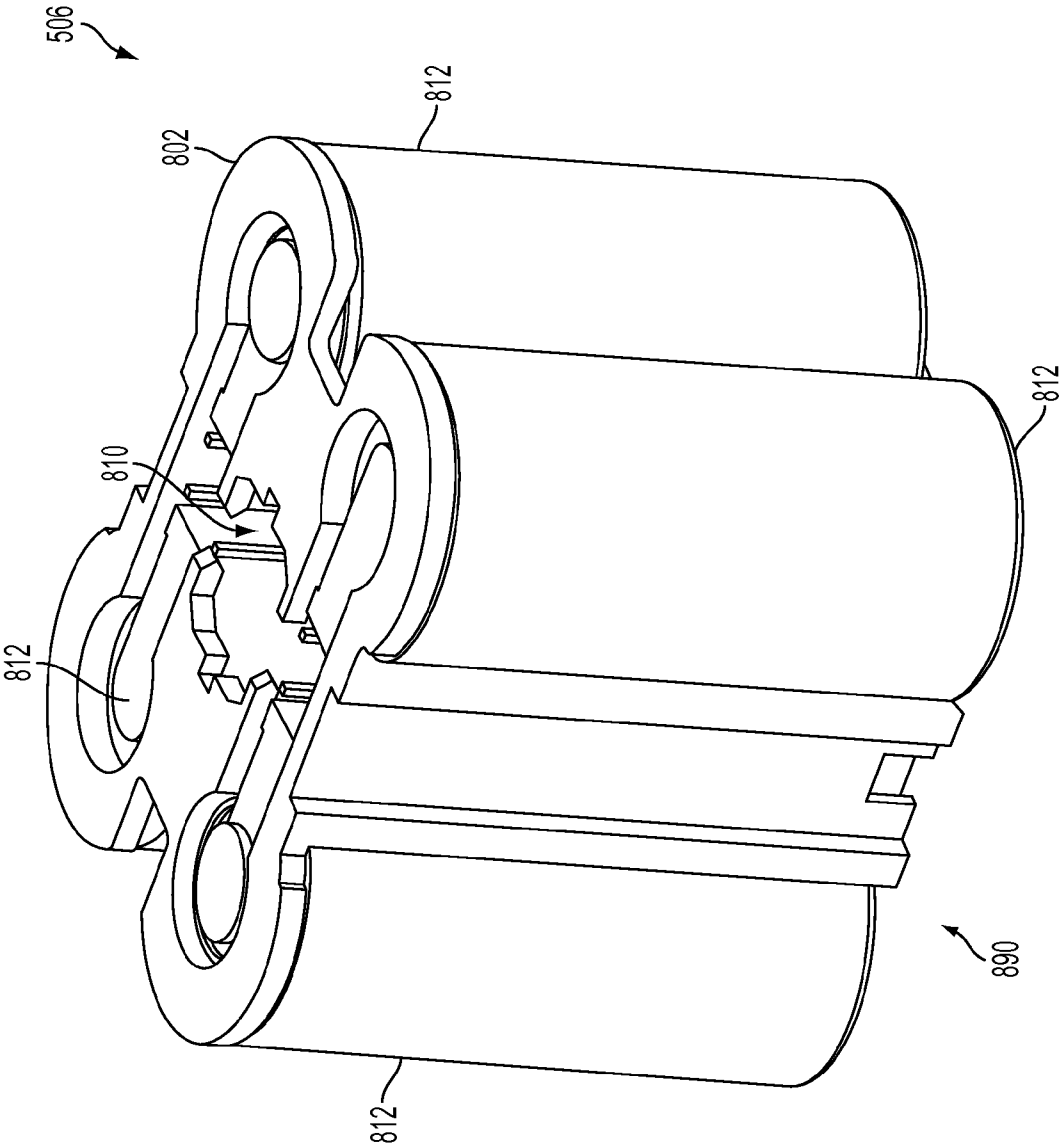


FIG. 35

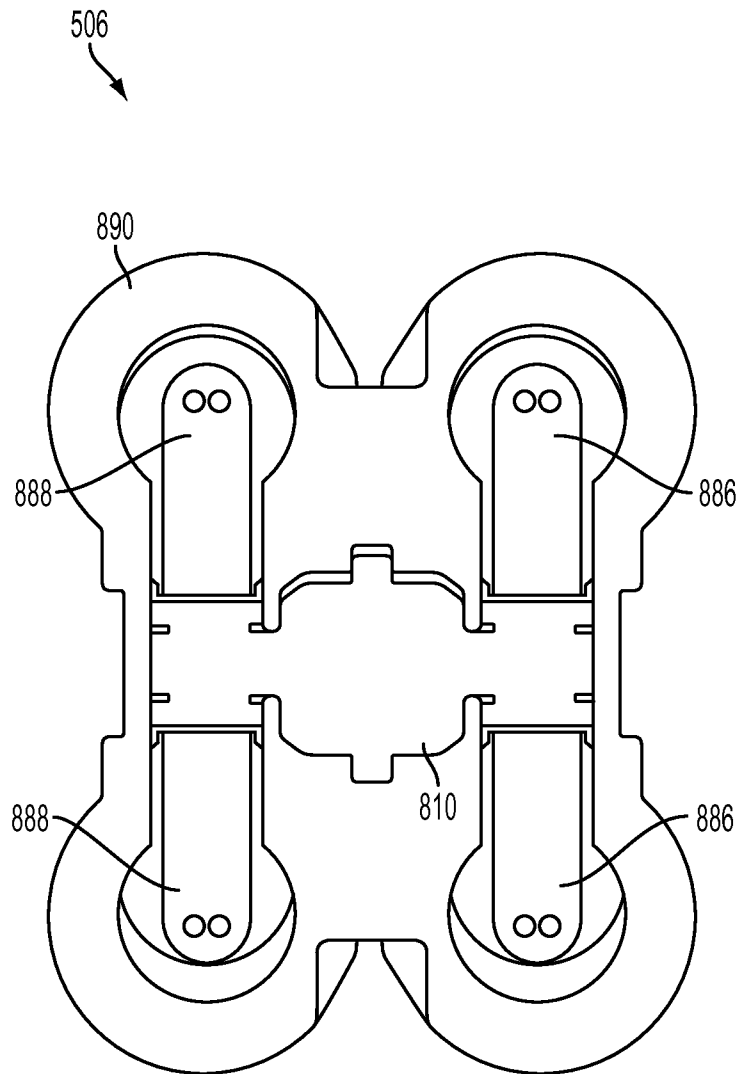


FIG. 36

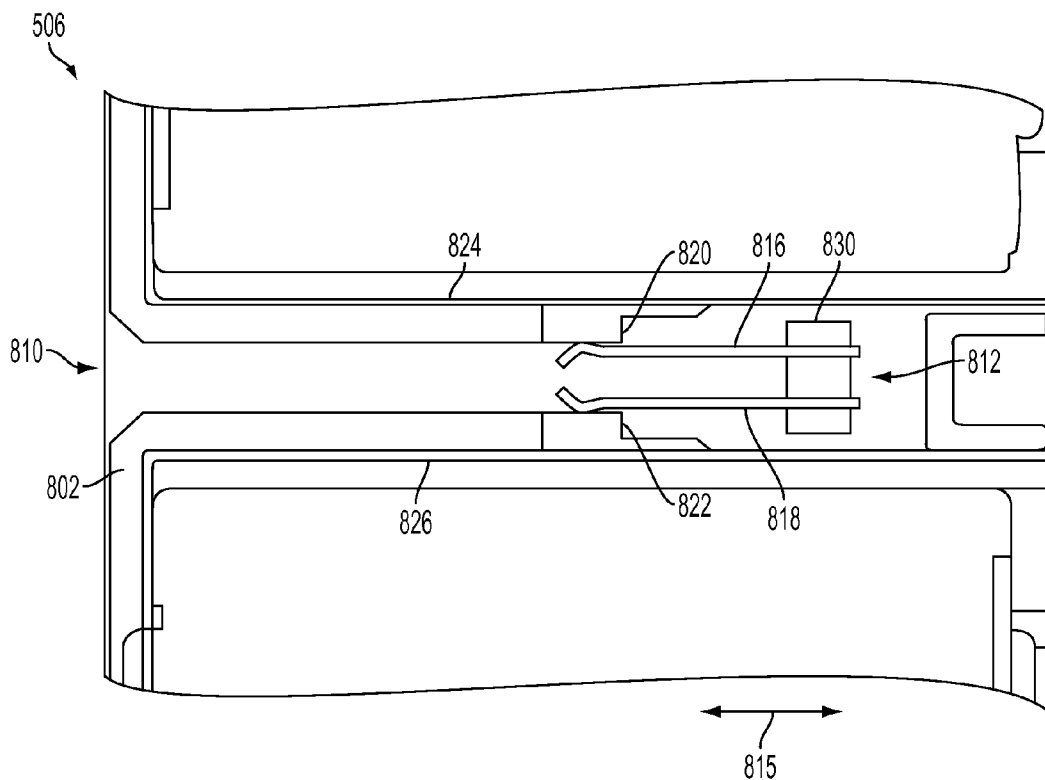


FIG. 37

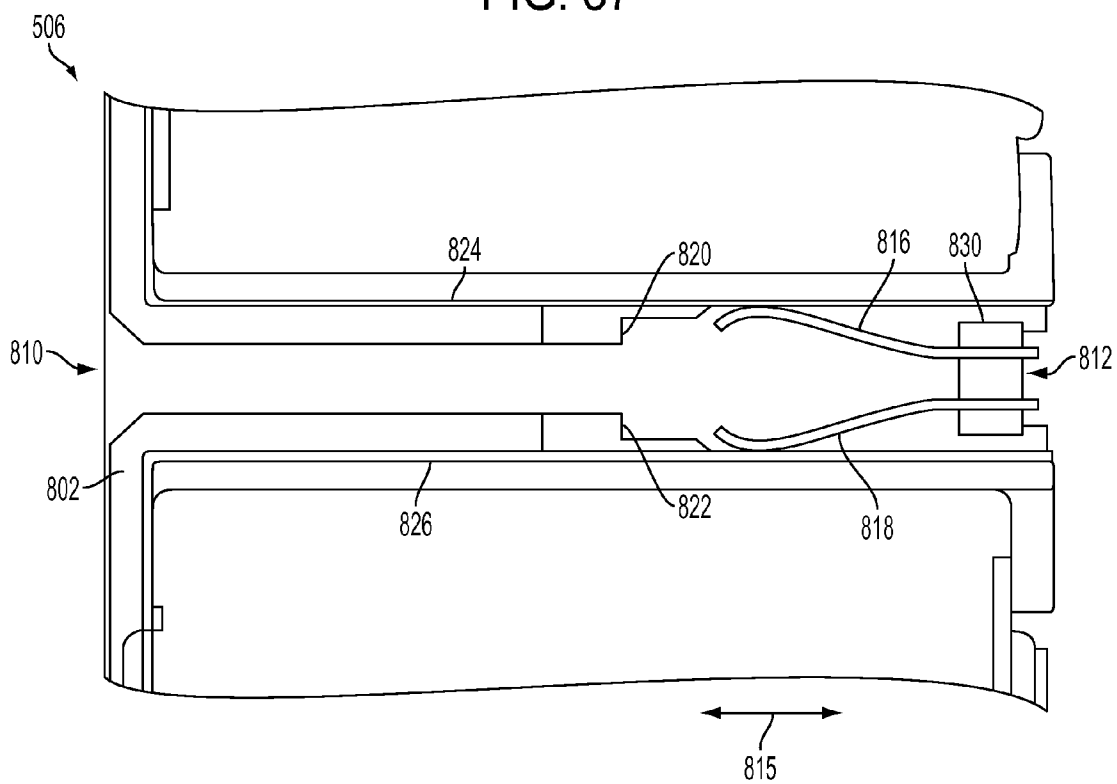


FIG. 38

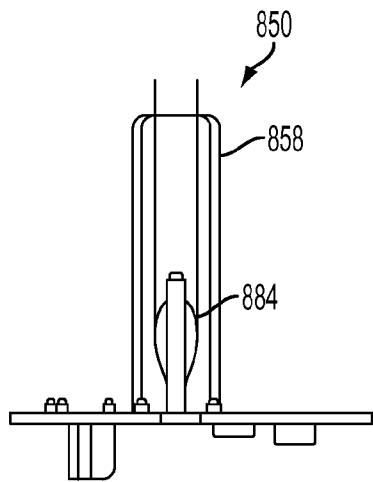


FIG. 39

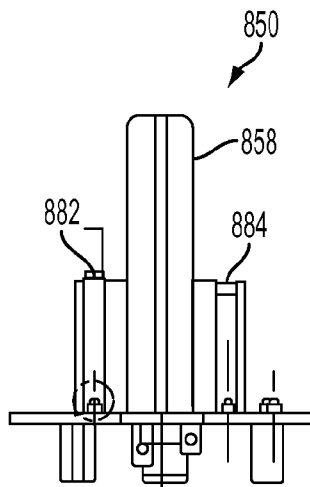


FIG. 40

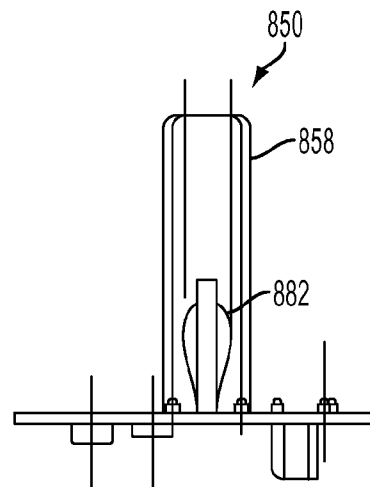


FIG. 41

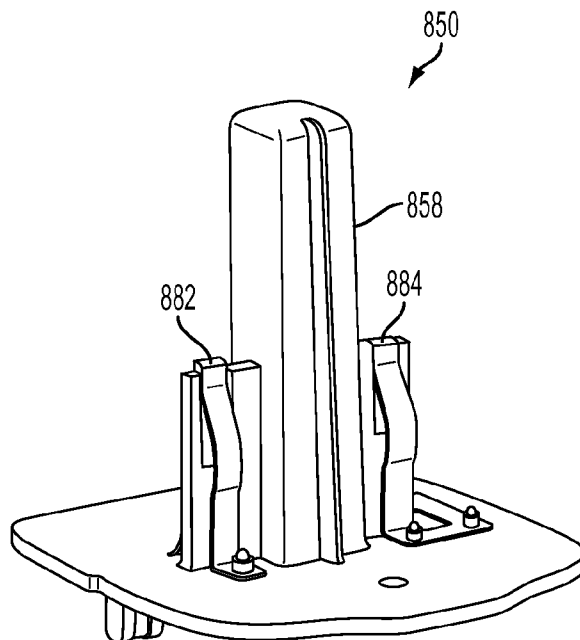


FIG. 42

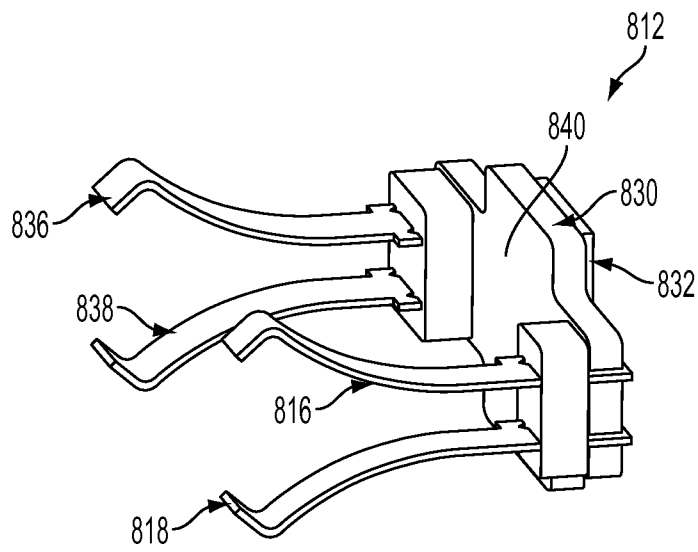


FIG. 43

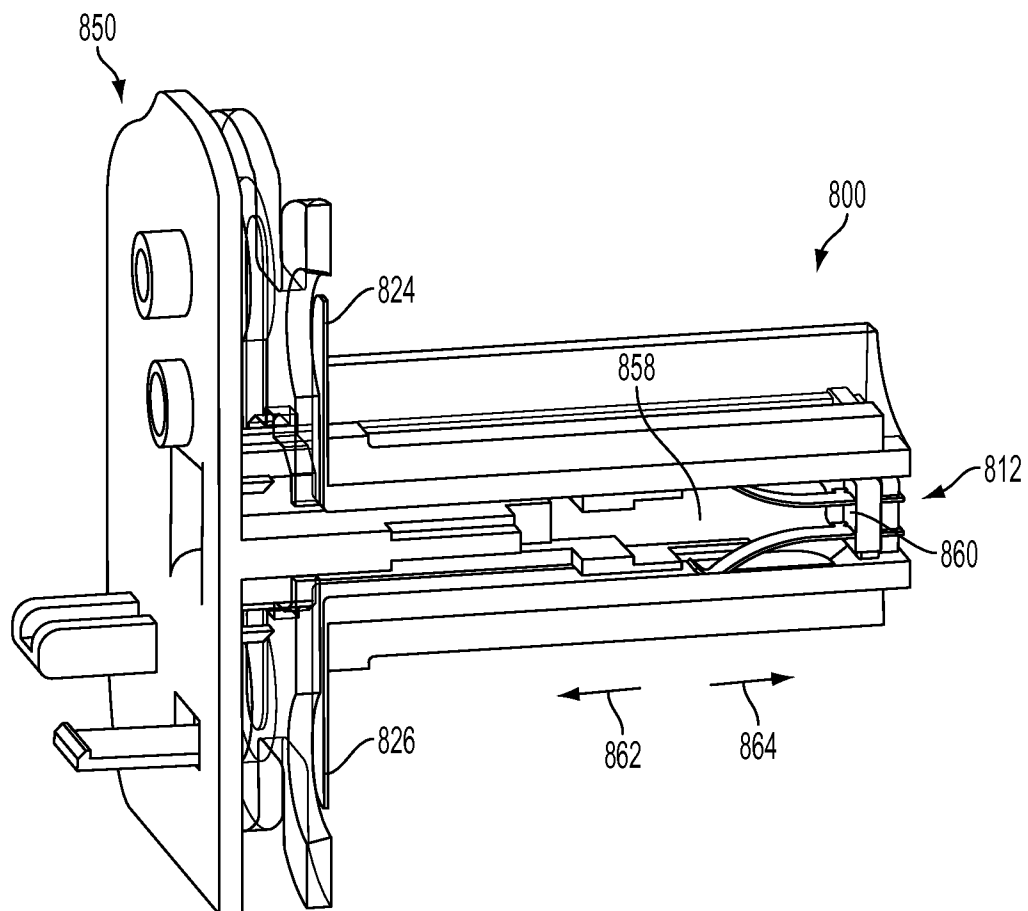


FIG. 44

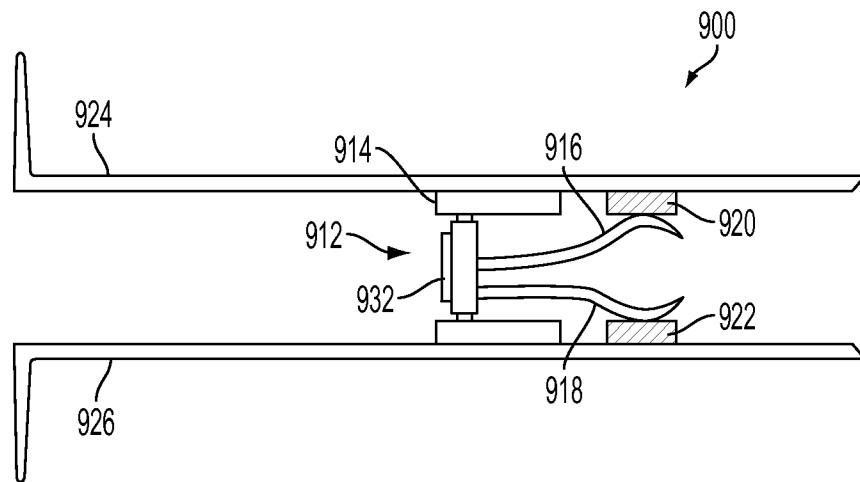


FIG. 45

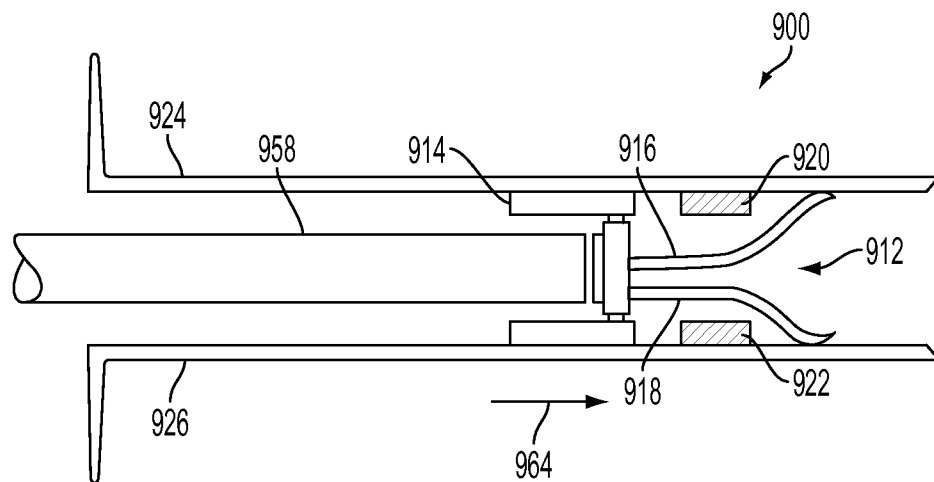


FIG. 46

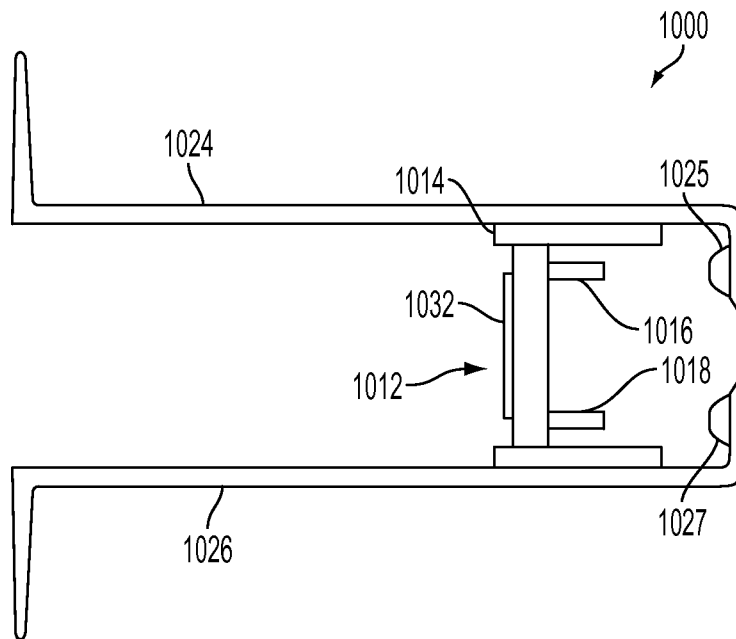


FIG. 47

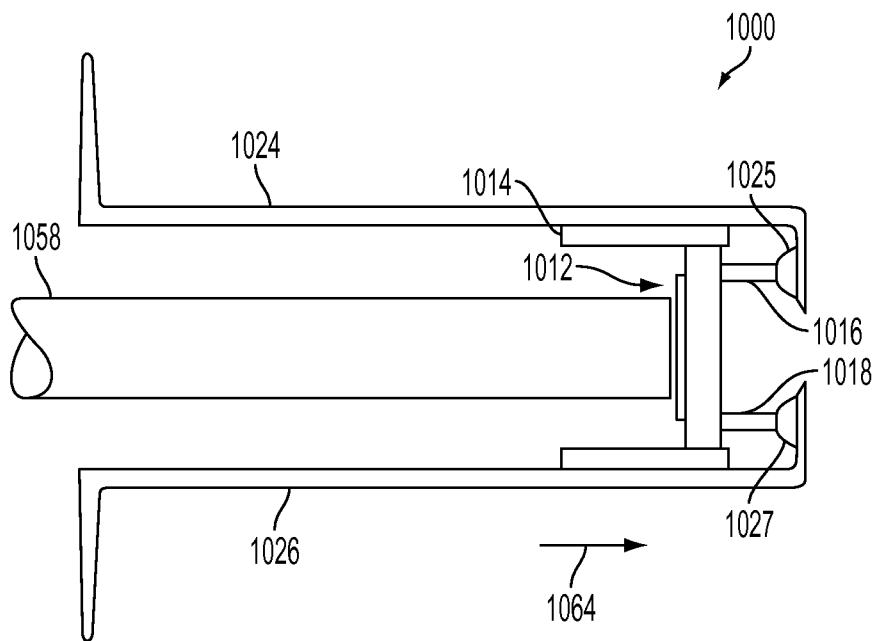


FIG. 48

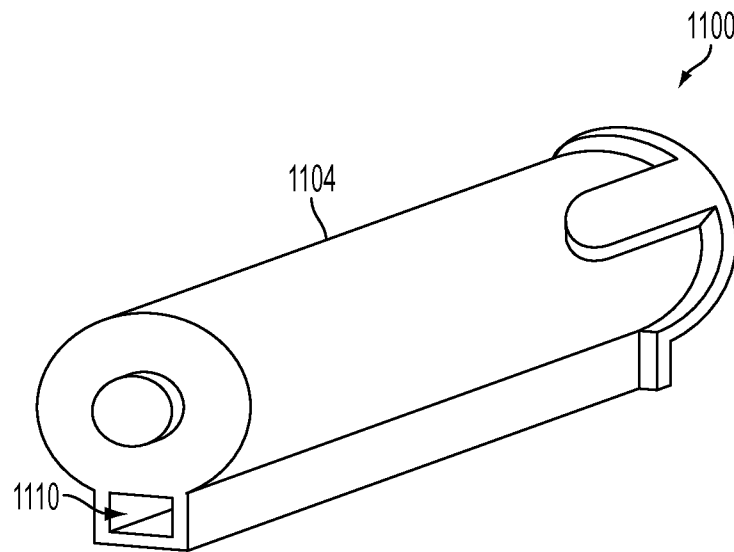


FIG. 49

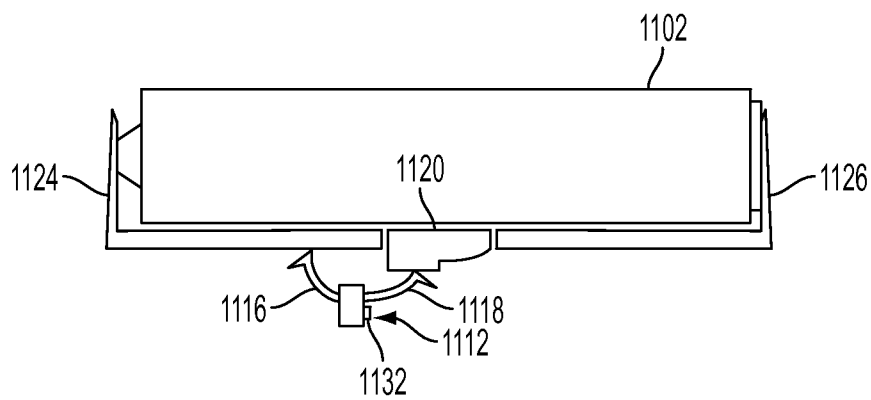


FIG. 50

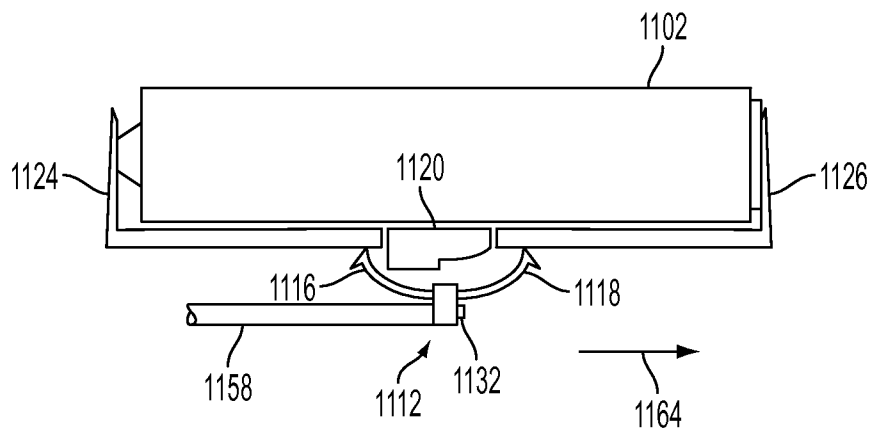


FIG. 51

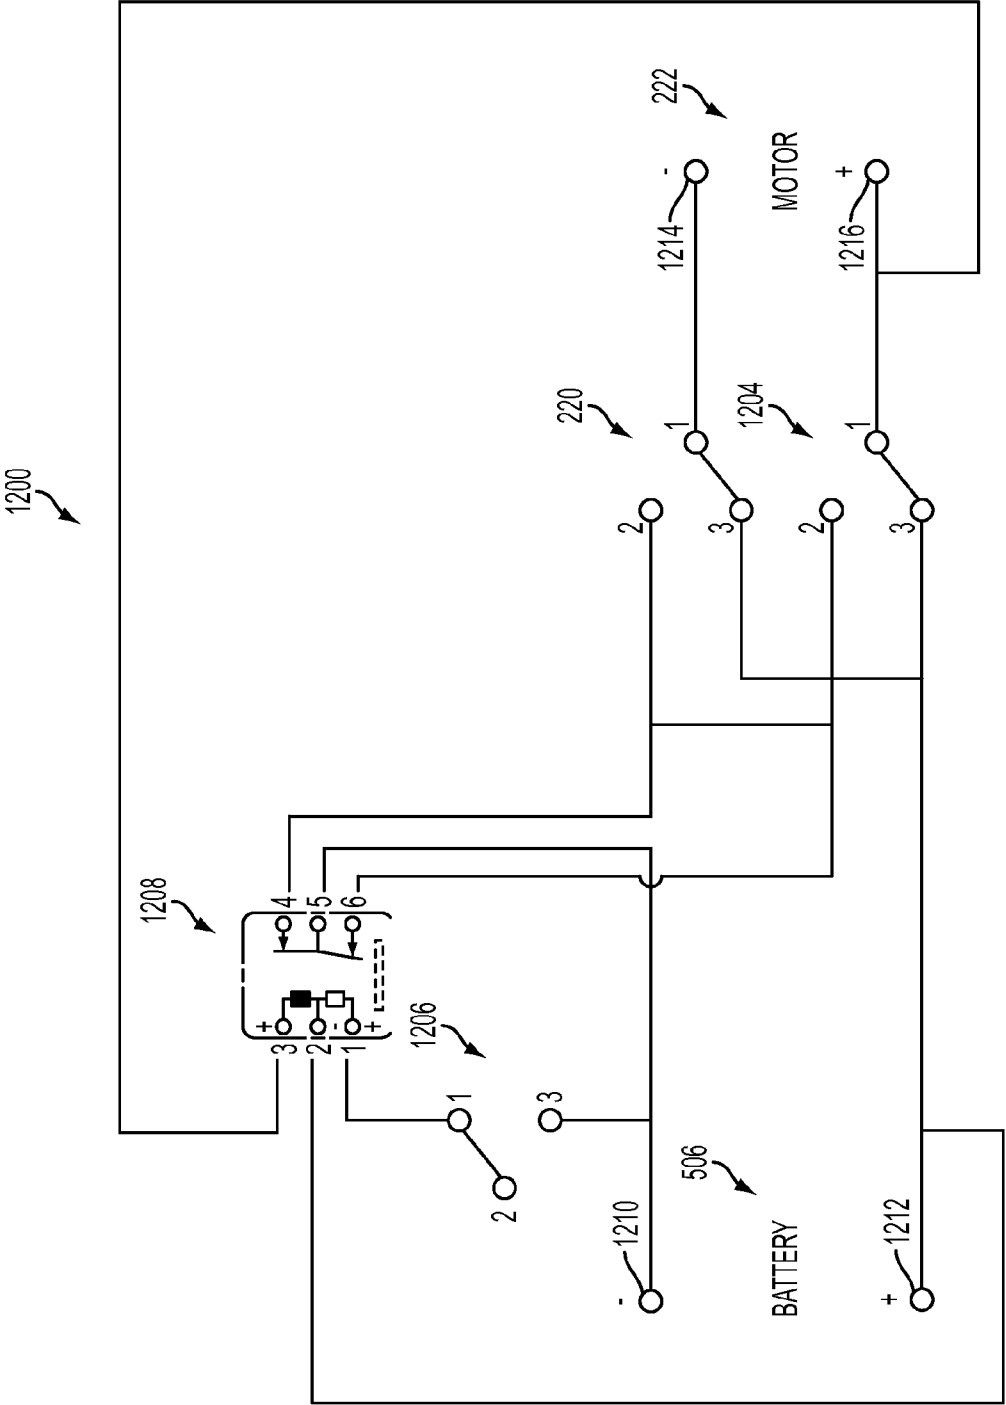


FIG. 52

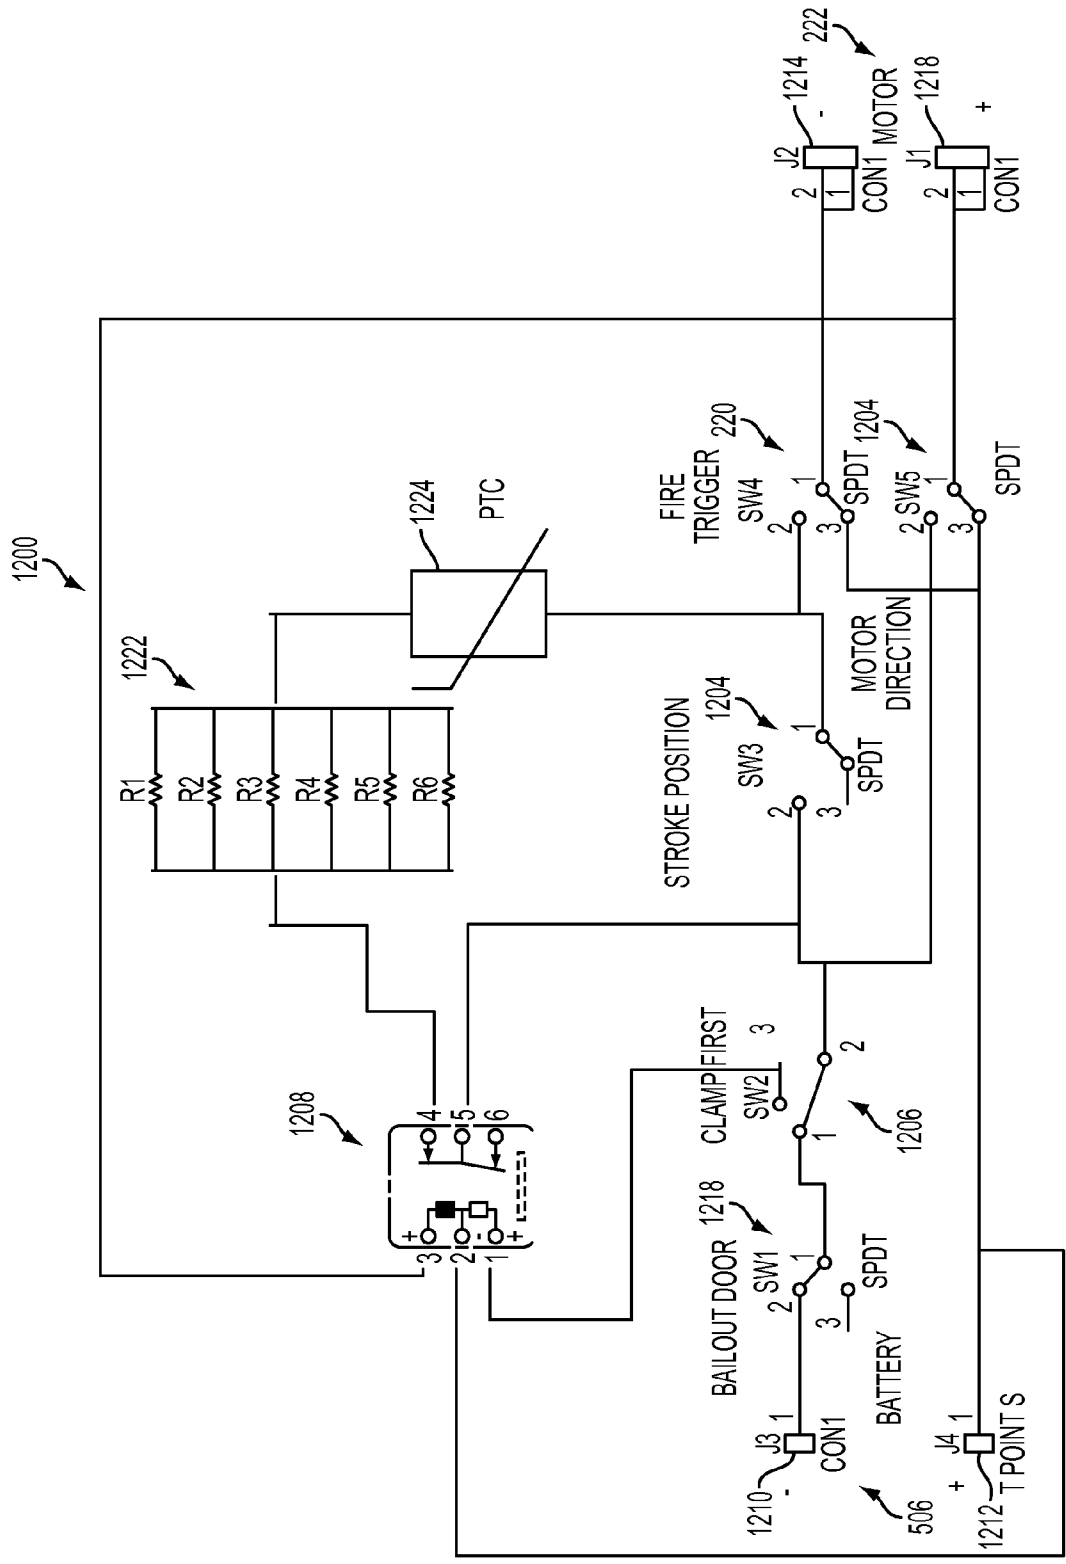


FIG. 53

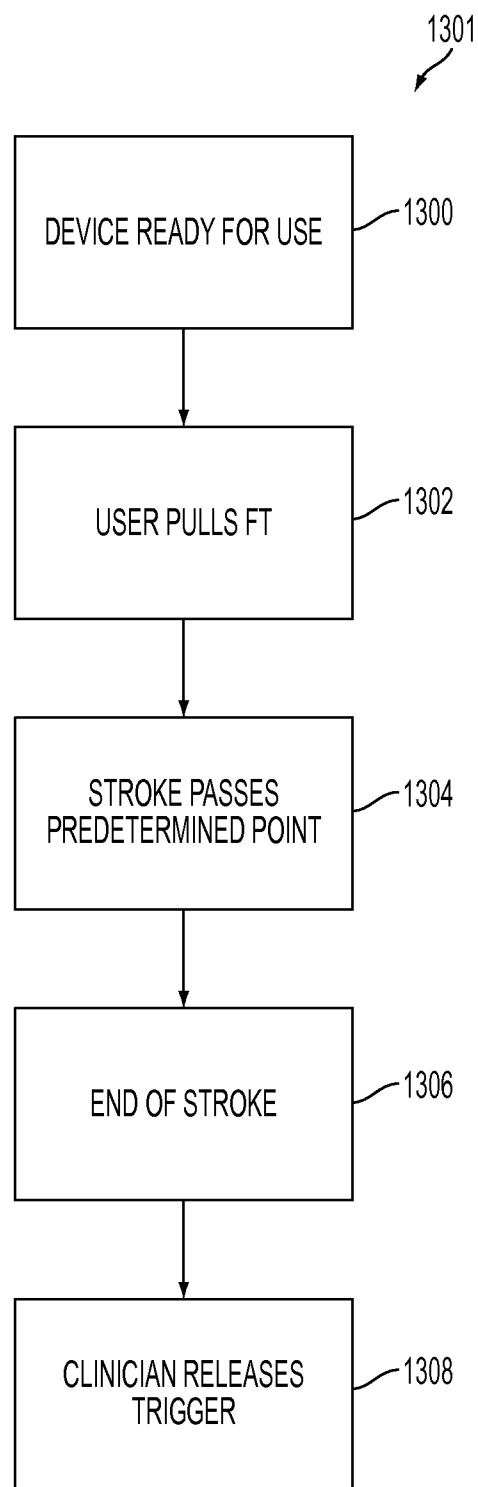


FIG. 54

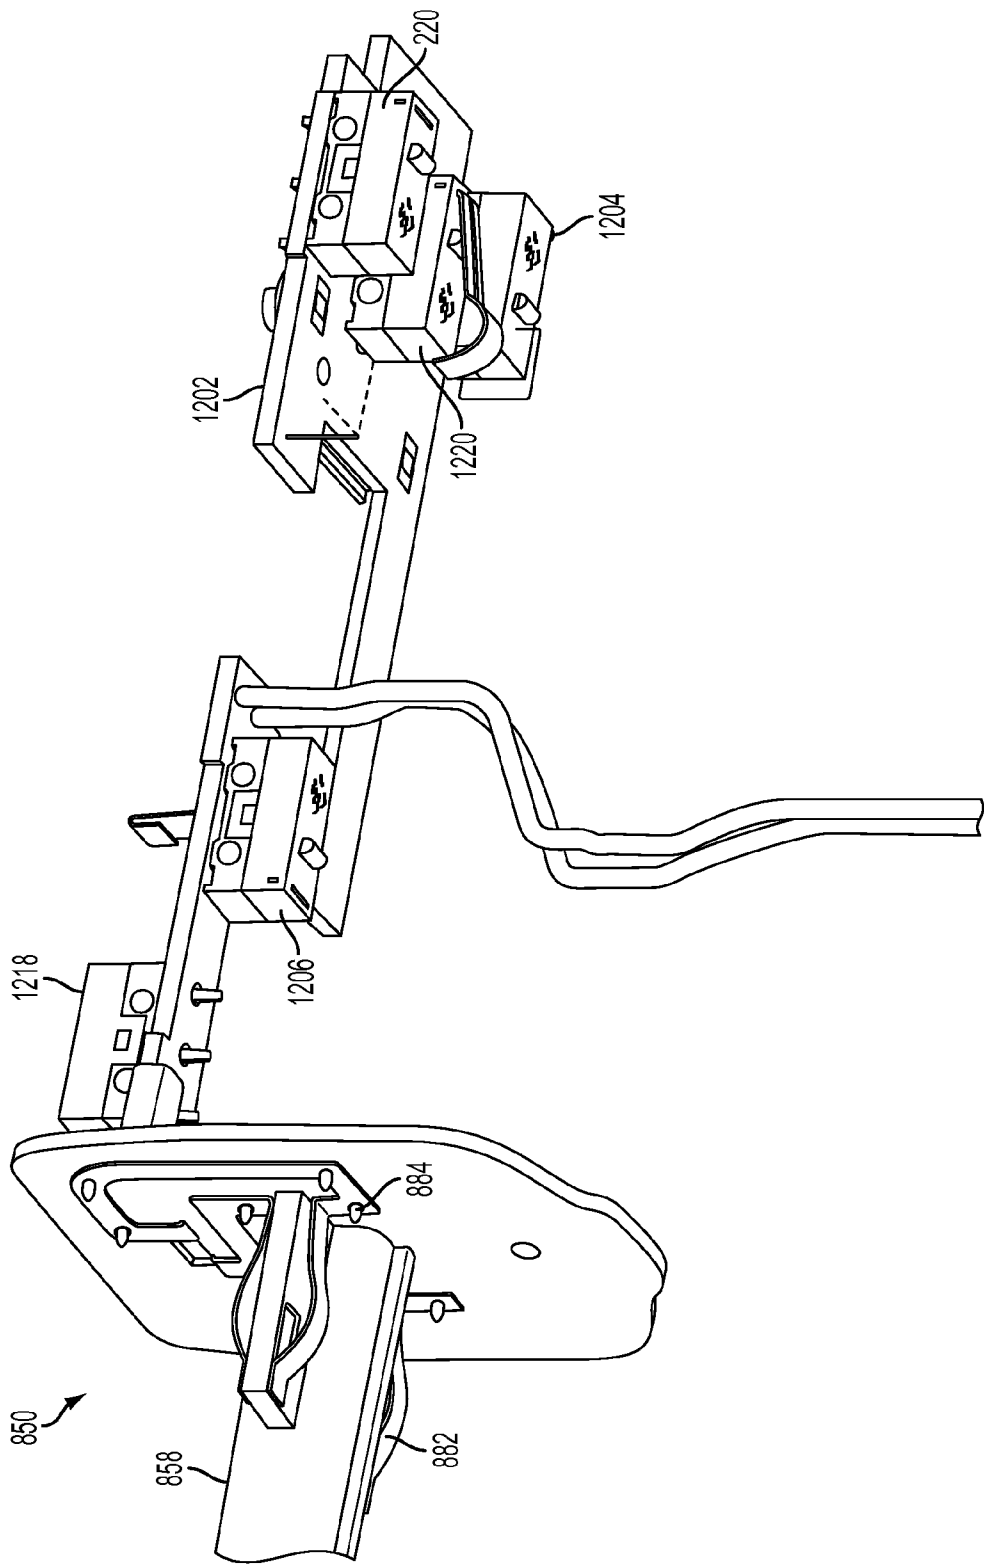


FIG. 55

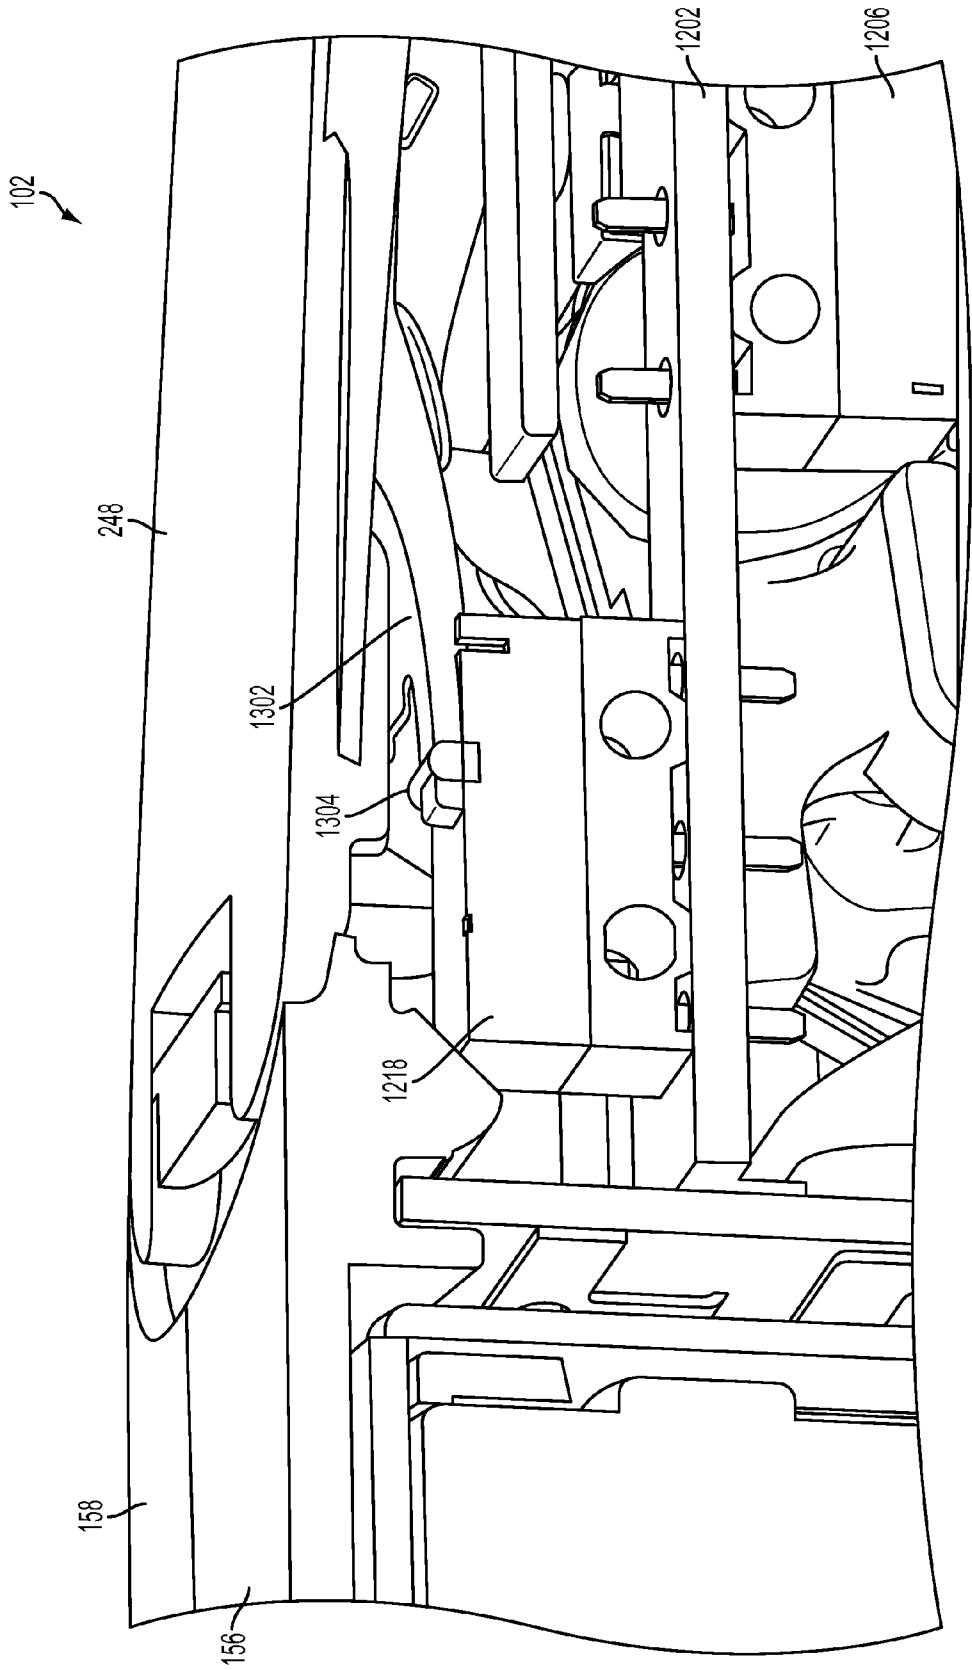


FIG. 56

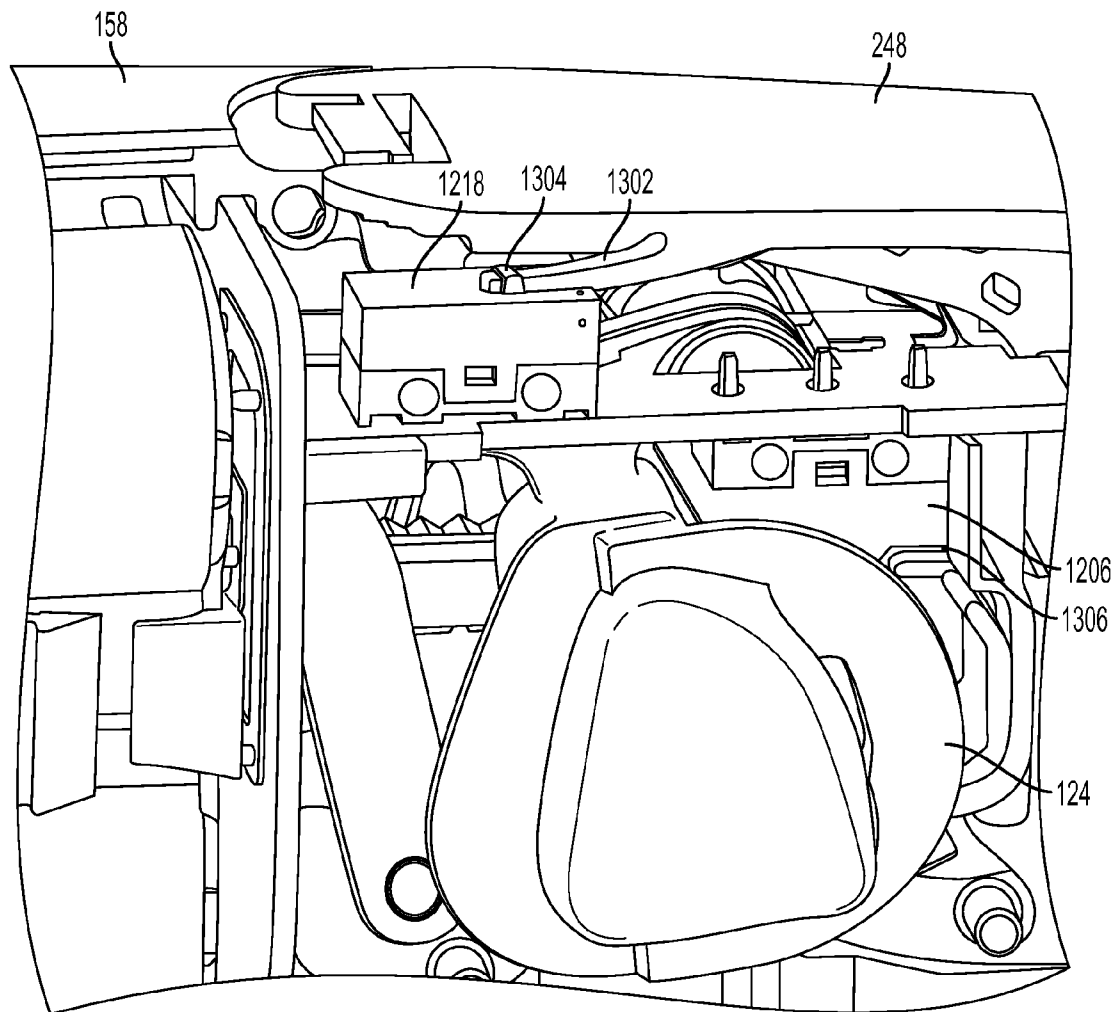


FIG. 57

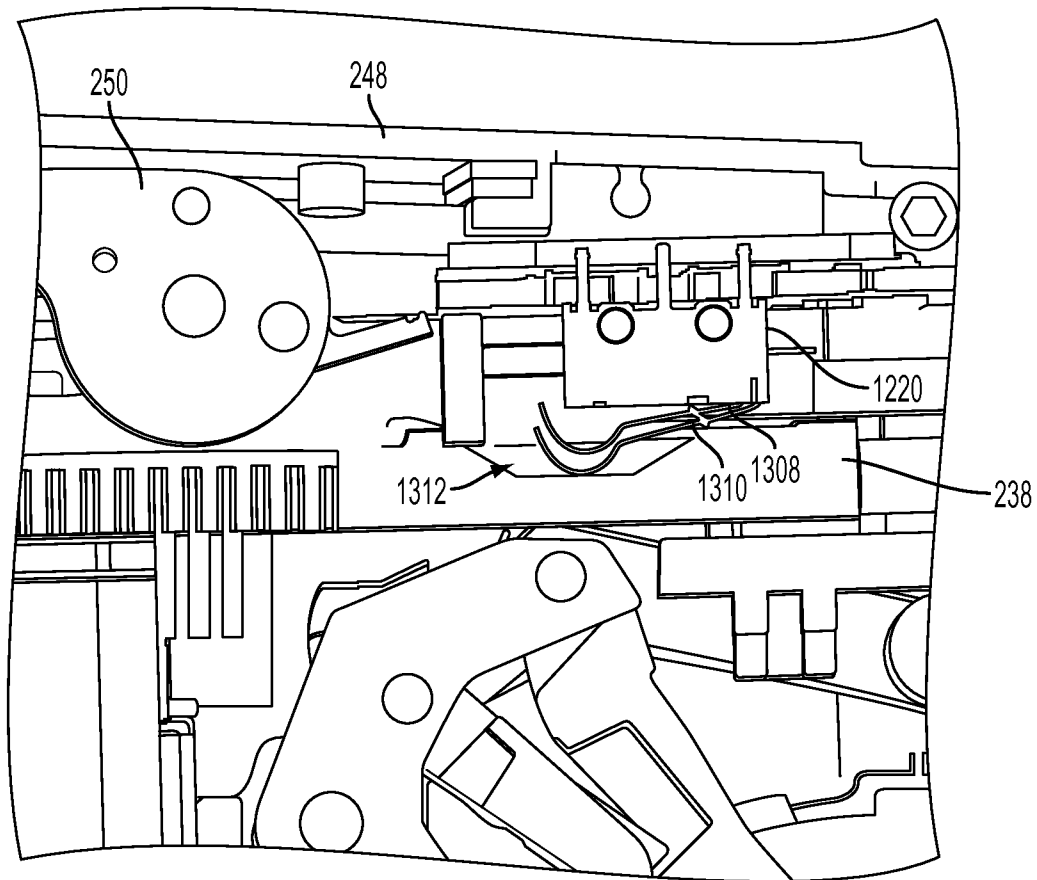


FIG. 58

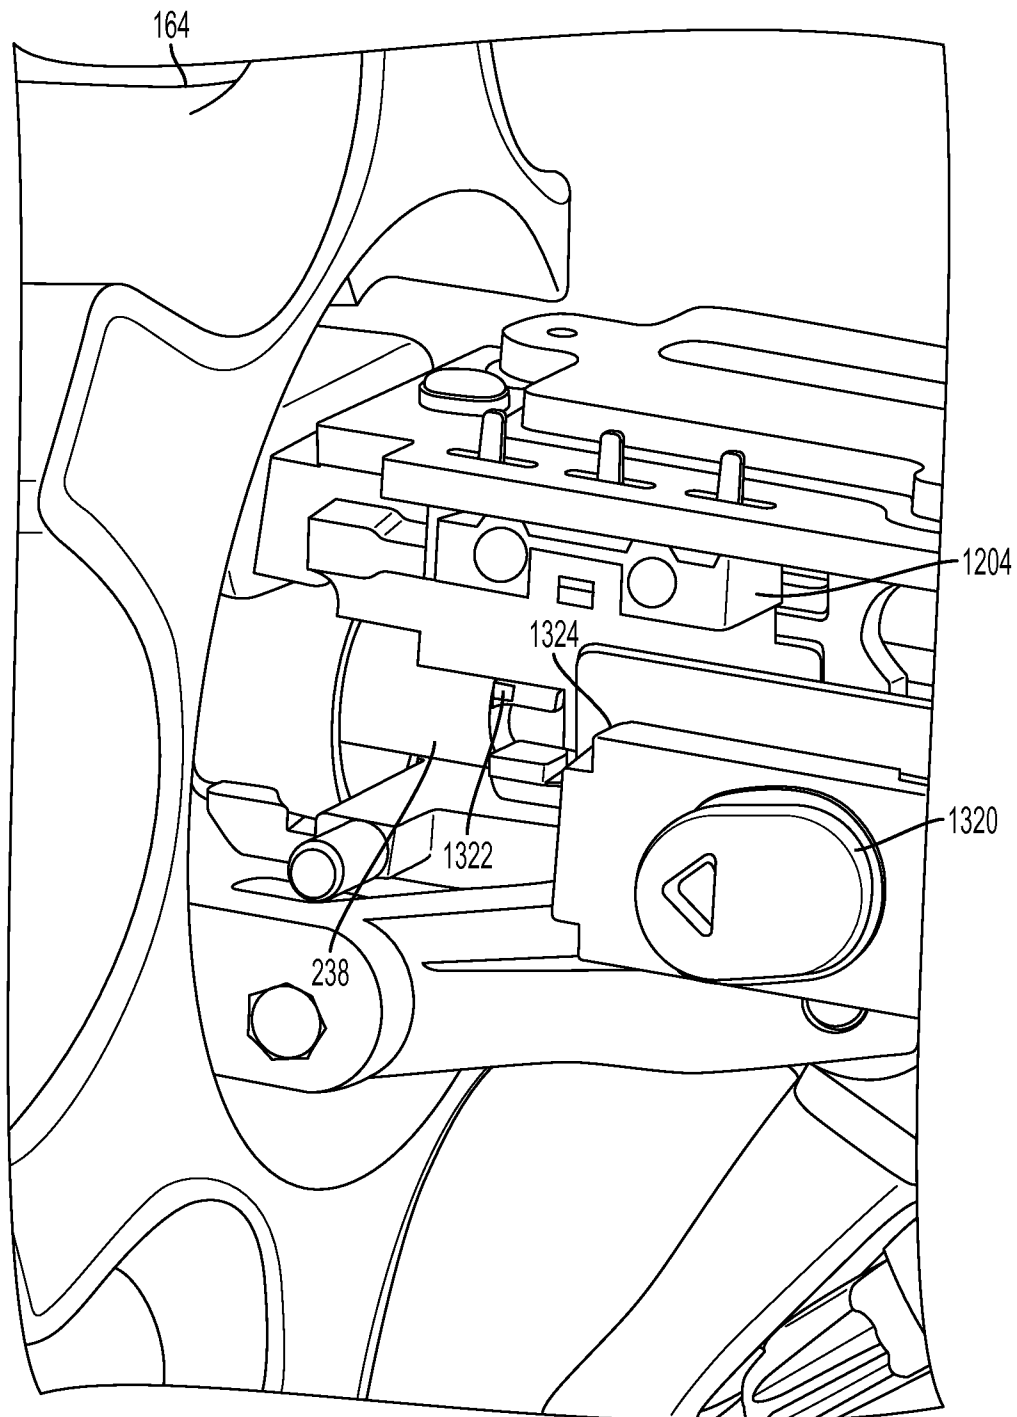


FIG. 59

1

SURGICAL INSTRUMENT HAVING A POWER CONTROL CIRCUIT

BACKGROUND

Traditionally, surgical devices have been hand operated, with the force to fire and/or manipulate the instruments provided directly by the clinician. A growing number of surgical instruments, however, are powered surgical instruments where the force to fire and/or manipulate the instrument are provided by an automated device, such as an electric motor, pneumatic or hydraulic device, etc. Examples of powered surgical instruments may include such as cutters, graspers, and/or staplers, for example. Such powered instruments free instrument designers from the need to limit the amount of force required to fire to that which can reasonably be provided by a human clinician. Powered instruments may also be more easily used by smaller clinicians and/or clinicians with less physical strength.

One significant challenge of powered instruments, however, is lack of feedback to the clinician. When a clinician uses a manually powered surgical instrument, the clinician is able to know the state of the instrument based on the amount of force that the clinician has already provided to the instrument, the position of the handle trigger or other device for receiving clinician force, etc. In a powered instrument, however, such feedback may be absent. Accordingly, there is a need to compensate for the lack of feedback from powered surgical instruments.

DRAWINGS

The features of the various embodiments are set forth with particularity in the appended claims. The various embodiments, however, both as to organization and methods of operation, together with advantages thereof, may best be understood by reference to the following description, taken in conjunction with the accompanying drawings as follows:

FIG. 1 shows one embodiment of a surgical stapling and cutting instrument with an electrically powered firing feature.

FIG. 2 shows one embodiment of an end effector of the instrument of FIG. 1.

FIGS. 3 and 4 show additional views of one embodiment of a firing bar of the instrument of FIG. 1.

FIG. 5 illustrates an alternative embodiment of an end effector having a firing bar lacking a middle pin.

FIG. 6 illustrates a cut-away side view of one embodiment of the surgical instrument of FIG. 1.

FIG. 7 illustrates an exploded view of one embodiment of the surgical instrument showing various components thereof.

FIG. 8 illustrates a shallower cut-away side view of one embodiment of the surgical instrument of FIG. 1 to show component features not shown in the cut-away side view of FIG. 6.

FIG. 9 illustrates an internal view of one embodiment of the surgical instrument of FIG. 1.

FIG. 10 illustrates a partial cross-sectional view of one embodiment of the surgical instrument of FIG. 1 with various components removed for clarity showing the operation of the retraction lever.

FIGS. 11 and 12 illustrate one embodiment of a locking cam of the surgical instrument of FIG. 1 during various states of operation.

FIGS. 13-15 show various embodiments of the locking cam of FIGS. 11 and 12 and a intermediate gear during three stages of operation.

2

FIG. 16 depicts one embodiment of the end effector of the instrument of FIG. 1 in an open position, as a result of a retracted closure sleeve, with a staple cartridge installed in the elongate channel.

FIG. 17 shows one embodiment of the implement portion of the surgical stapling and severing instrument of FIG. 1 in disassembled form.

FIG. 18 shows one embodiment of the end effector of the instrument of FIG. 1 with a portion of the staple cartridge removed.

FIG. 19 depicts the end effector of FIG. 18 with all of the staple cartridge removed.

FIG. 20 depicts one embodiment of the end effector of the instrument of FIG. 1 closed in a tissue clamping position with the firing bar unfired.

FIG. 21 depicts one embodiment of the upper surface of the staple cartridge shown in FIG. 16 with the firing bar in its unfired, proximal position.

FIG. 22 depicts one embodiment of the end effector of the instrument of FIG. 1 near the pivot showing that the elongate channel has opposing ramp portions to thereby cooperate with the anvil to prevent tissue from jamming the end effector.

FIG. 23 illustrates one embodiment of the end effector of the instrument of FIG. 1 with tissue present between the staple cartridge and the anvil.

FIGS. 24-26 illustrate one embodiment of the end effector of the instrument of FIG. 1 at various stages of firing.

FIGS. 27-29 schematically illustrate one embodiment of a battery unit and a portion of the instrument of FIG. 1 showing the attachment and detachment of the battery unit to the instrument.

FIG. 30 illustrates a graph of the voltage level of one embodiment of the battery unit of FIGS. 27, 28 and 29 over time, as measured from the time of attachment to the instrument of FIG. 1.

FIG. 31 shows one embodiment of a simplified circuit diagram of one embodiment of a battery unit comprising a drain.

FIG. 32 is one embodiment of a simplified circuit diagram of one embodiment of a battery unit comprising a first drain and a second drain.

FIGS. 33-36 are perspective views of one embodiment of a battery unit.

FIGS. 37 and 38 illustrate cross-sectional views of one embodiment of the battery unit of FIGS. 33-36 including a translatable drain.

FIGS. 39-42 show multiple views of one embodiment of a battery dock.

FIG. 43 is a perspective view of one embodiment of the translatable drain of FIGS. 37 and 38.

FIG. 44 illustrates one embodiment of the battery unit of FIGS. 33-36 attached to a battery dock with various components omitted for clarity.

FIGS. 45 and 46 illustrate one embodiment of a battery unit with various components omitted for clarity.

FIGS. 47 and 48 illustrate one embodiment of a battery unit with various components omitted for clarity.

FIG. 49 is a perspective view of one embodiment of single cell battery unit.

FIGS. 50 and 51 show internal views of the battery unit of FIG. 49 during various stages of operation with various components omitted for clarity.

FIG. 52 illustrates one embodiment of a control circuit that may control a connection between the battery unit or other power supply and the motor or other drive device for firing the instrument of FIG. 1.

3

FIG. 53 illustrates one embodiment of the control circuit of FIG. 52 with additional switches and features.

FIG. 54 is a flowchart showing one embodiment of a process flow showing the firing of the instrument of FIG. 1 utilizing the control circuit as illustrated in FIG. 53.

FIG. 55 illustrates a perspective view of one embodiment of circuit board for implementing the control circuit of FIG. 52 or 53, coupled to the battery dock of FIG. 36.

FIG. 56 illustrates a cut away view of one embodiment of the instrument of FIG. 1 showing the emergency access door switch.

FIG. 57 illustrates another cut away view of one embodiment of the instrument of FIG. 1 showing the clamp switch.

FIG. 58 illustrates another cut away view of one embodiment of the instrument of FIG. 1 showing the stroke position switch.

FIG. 59 illustrates another cut away view of one embodiment of the instrument of FIG. 1 showing the end-of-stroke/motor reverse switch.

DESCRIPTION

Various embodiments are directed to surgical instruments having control circuits for implementing an electronic lock-out. For example, the control circuit may comprise one or more latching devices such as, for example, a latching relay, a transistor, etc. The surgical devices may comprise an end effector having first and second jaw members, where at least one of the jaw members is translatable (e.g., pivotally or otherwise) towards the other. The surgical instruments may also have a firing bar that is translatable through the end effector when the jaw members are closed (e.g., pivoted towards one another). The jaw members of the end effector may serve to clamp tissue. Once tissue is clamped, the firing bar may act upon the tissue. In various embodiments, distal motion of the firing bar may cause cutting and/or fastening of tissue. For example, the firing bar may define a cutting edge or knife to cut tissue clamped between the jaw members. Also, for example, the firing bar may drive a wedge or other mechanism to drive staples through the tissue clamped between the jaw members. According to various embodiments, the firing bar may be driven by a drive device such as, for example, an electric motor, a pneumatic or hydraulic device, etc. The drive device may be powered by a power supply such as, for example, a battery and/or a connection to an external source of electrical power, such as a wall outlet.

FIG. 1 shows one embodiment of a surgical stapling and cutting instrument 102 with an electrically powered firing feature. The illustrated embodiment is an endoscopic instrument and, in general, the embodiments of the instrument 102 described herein are endoscopic surgical cutting and fastening instruments. It should be noted, however, that according to other embodiments, the instrument may be a non-endoscopic surgical cutting and fastening instrument, such as a laparoscopic or open surgical instrument. The instrument 102 may comprise an end effector 104 that may be operative to staple and cut tissue in response to control operations executed by a clinician grasping a handle portion 106. FIG. 2 shows one embodiment of the end effector 104 of the instrument 102. According to various embodiments, the instrument 102 may utilize an E-beam firing mechanism or firing bar 108 that may control the spacing of the end effector 104. For example, a first jaw member, or elongate channel 110 and a pivotally translatable second jaw member or anvil 112 may be maintained at a spacing that assures effective stapling and severing.

4

The instrument 102 may comprise the handle portion 106 and an implement portion 114. The implement portion 114 may be connected to the handle portion 106 and may comprise a shaft 116 distally terminating in the end effector 104.

The handle portion 106 may comprise a pistol grip 118. A closure trigger 120 may be positioned such that a clinician may pivotally draw the closure trigger 120 towards the pistol grip 118 to cause clamping, or closing, of the anvil 112 toward the elongate channel 110 of the end effector 104. A firing trigger 122 may be positioned farther outboard of the closure trigger 120 and may be pivotally drawn by the clinician to cause the stapling and severing of clamped tissue in the end effector 104. As described below, the stapling and severing of the clamped tissue by the end effector 104 may be powered by an electric motor.

It will be appreciated that the terms “proximal” and “distal” are used herein with reference to a clinician gripping a handle of an instrument. Thus, the end effector 104 is distal with respect to the more proximal handle portion 106. It will be further appreciated that for convenience and clarity, spatial terms such as “vertical” and “horizontal” are used herein with respect to the drawings. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and absolute.

In use, the clinician may actuate the closure trigger 120 first. For example, once the clinician is satisfied with the positioning of the end effector 104, the clinician may draw back the closure trigger 120 to its fully closed, locked position proximate to the pistol grip 118. Then, the clinician may actuate the firing trigger 122 to initiate powered cutting and stapling of tissue held between the anvil 112 and elongate channel 110. For example, the firing bar 108 may be powered forward to cut tissue and drive staples, for example, as described herein below. When the clinician removes pressure from the firing trigger 122, the firing bar 108 may be returned to the pre-firing position shown in FIG. 2. The clinician may actuate a release button 124 on the handle portion 106 to release the closure trigger 120. The clinician may then release the closure trigger, in turn releasing the anvil 112 and elongate channel 110 to pivot away from one another back to the position shown in FIG. 2.

Referring again to FIG. 1, the shaft 116 may comprise a frame 126 enclosed by a closure sleeve 128. A firing drive member 130 may be positioned within the frame 126 and may extend from the handle portion 106 to the firing bar 108. The drive member 130 may comprise a single component, or may be made up of multiple components. The frame 126 may connect the handle portion 106 to the end effector 104. With the closure sleeve 128 withdrawn proximally by the closure trigger 120 as depicted in FIGS. 1 and 2, the anvil 112 may springedly open, pivoting away from the elongate channel 110 and translating proximally with the closure sleeve 128.

The elongate channel 110 may receive a staple cartridge 132 that may be responsive to the firing bar 108 to drive staples into forming contact with the anvil 112. It will be appreciated that although a readily replaceable staple cartridge 132 is advantageously described herein, a staple cartridge 132 consistent with various embodiments may be permanently affixed or integral to the elongate channel 110, for instance when a larger portion of the end effector 104 is replaced after each firing.

FIGS. 3 and 4 show additional views of one embodiment of the firing bar 108. As illustrated in FIGS. 2-4, the firing bar 108 may include three vertically spaced pins that control the spacing of the end effector 104 during firing. An upper pin 134 may be staged to enter an anvil pocket 136 near the pivot between the anvil 112 and elongate channel 110. When fired

5

with the anvil 112 closed, the upper pin 134 may advance distally within a longitudinal anvil slot 138 extending distally through anvil 112. According to various embodiments, minor upward deflections of the anvil 112 may be overcome by a downward force imparted on the anvil 112 by the upper pin 134. The firing bar 108 may also include a lower pin, or firing bar cap, 140 that may upwardly engage a channel slot 142 in the elongate channel 110, thereby cooperating with the upper pin 134 to draw the anvil 112 and the elongate channel 110 together in the event of excess tissue clamped therebetween.

The firing bar 108 may also comprise a middle pin 144 that may pass through a firing drive slot 146 formed in a lower surface of the cartridge 132 and an upward surface of the elongate channel 110. In this way, the middle pin 144 may initiate the driving of the staples, as described below. The middle pin 144, by sliding against the elongate channel 110, may resist a tendency for the end effector 104 to be pinched shut at its distal end. To illustrate an advantage of the middle pin 144, FIG. 5 illustrates an alternative embodiment of an end effector 148 having a firing bar 150 lacking a middle pin. As shown in FIG. 5, the end effector 148 is allowed to pinch shut at its distal end, which may tend to impair desired staple formation.

Returning to FIGS. 2-4, the firing bar 108 may comprise a distally presented cutting edge 152 between the upper and middle pins 134, 144. When the end effector 104 is fired, the cutting edge 152 may traverse through a proximally presented, vertical slot 154 in the cartridge 132 to sever clamped tissue present between the anvil 112 and the elongate channel 110. The affirmative positioning of the firing bar 108 with regard to the elongate channel 110 and anvil 112 may make it more likely that an effective cut is performed.

The affirmative vertical spacing provided by the E-Beam firing bar 108 may be suitable for the limited size available for endoscopic devices. Moreover, the E-Beam firing bar 108 may enable fabrication of an anvil 112 with a camber imparting a vertical deflection at its distal end, similar to the position depicted in FIG. 5. This cambered anvil 112 may assist in achieving a desirable gap in the end effector 104 even with an anvil 112 having reduced thickness, which may be thus more suited to the size limitations of an endoscopic device. The E-Beam firing bar 108 may further enable increased applications, especially in combination with a range of configurations of staple cartridges. For instance, a clinician may select a gray staple cartridge yielding a 0.02 mm tissue gap, a white staple cartridge yielding a 0.04 mm tissue gap, a blue cartridge yielding a 0.06 mm tissue gap, or a green cartridge yielding a 0.102 mm tissue gap. The vertical height of each respective staple cartridge in combination with the length of staples and an integral wedge sled (described in more detail below) may predetermine this desired tissue thickness with the anvil 112 appropriately vertically spaced by the E-Beam firing bar 108.

FIGS. 6-9 illustrate various internal components of the handle portion 106 of one embodiment of the surgical instrument 102. For example, FIG. 6 illustrates a cut-away side view of one embodiment of the surgical instrument 102. FIG. 7 illustrates an exploded view of one embodiment of the surgical instrument 102 showing a portion of the components thereof. FIG. 8 illustrates a cut-away side view of one embodiment of the surgical instrument of 102 that is shallower than the cut-away of FIG. 6 in order to show component features not shown in the cut-away side view of FIG. 6. FIG. 9 illustrates an internal view of one embodiment of the surgical instrument 102.

With reference to FIGS. 6-9, the handle portion 106 may be comprised of first and second base sections 156 and 158,

6

which may be molded from a polymeric material such as a glass-filled polycarbonate. Within the first and second base sections 156, 158 may be first and second frame sections 160, 162. A rotating knob 164 may have a bore 166 extending completely through it for engaging and rotating the implement portion 114 about its longitudinal axis. The rotating knob 164 may include an inwardly protruding boss 168 extending along at least a portion of the bore 166. The protruding boss 168 is received within a longitudinal slot 170 formed at a proximal portion of the closure sleeve 128 such that rotation of the rotating knob 164 effects rotation of the closure sleeve 128. It will be appreciated that the boss 168 may further extend through frame 126 and into contact with a portion of the firing drive member 130 to effect its rotation as well. Thus, the end effector 104 may rotate with the rotating knob 164.

A proximal end 172 of the frame 126 may pass proximally through the rotating knob 164 and may be provided with a circumferential notch 174 that is engaged by opposing channel securement members 176 extending respectively from the frame sections 160 and 162. The channel securement members 176 extending from the frame sections 160, 162 may serve to secure the frame 126 to the handle portion 106 such that the frame 126 does not move longitudinally relative to the handle portion 106.

The closure trigger 120 may have a handle section 178, a lever section 180, and an intermediate section 182. A bore 184 may extend through the intermediate section 182. A cylindrical support member 186 may pass through the bore 184 for pivotally mounting the closure trigger 120 on the handle portion 106 (e.g., via the frame sections 160, 162). A second cylindrical support member 188 may pass through a bore 190 of firing trigger 122 for pivotally mounting the firing trigger 122 on the handle portion 106.

A closure yoke 192 may be housed within the handle portion 106 for reciprocating movement therein and serves to transfer motion from the closure trigger 120 to the closure sleeve 128. The closure yoke 192 may be coupled to the handle portion 106 via the respective frame portions 160, 162. A proximal end 194 of the closure sleeve 128 is provided with a flange 196 that is snap-fitted into a receiving recess 198 formed in the yoke 192. A distal end of the yoke 192 may be coupled to a secondary yoke 200 via a biasing member such as a spring 202. A proximal end of the yoke 192 may define a bore 204 for receiving a linkage 206. A proximal end of the linkage 206 may be coupled to the closure trigger 120. For example, the linkage 206 may comprise a bore for receiving the pin 188. In this way, when the clinician moves the handle section 178 of the closure trigger 120 proximally toward the pistol grip 118, the linkage 206 may be pushed distally, causing corresponding distal motion of the secondary yoke 200, compressing the spring 202 biases the yoke proximally and, in turn, pushing the yoke 192 and closure sleeve 128 distally. Distal movement of the closure sleeve 128 may cause pivotal translation movement of the anvil 112 distally and toward the elongate channel 110 of the end effector 104 and proximal movement effects closing, as described below.

As the closure trigger 120 is pulled towards the pistol grip 118, the lever portion 180 of the trigger 120 may translate distally. When the closure trigger 120 is fully pulled against the pistol grip 118, a clamp lock switch 124 may pivot about a clamp lock pin 208 to lock the closure trigger 120 into the clamped position. For example, the clamp lock switch 124 may be biased by a spring (not shown) to pivot about the pin 208. The clinician may unlock the closure trigger 120, for example, by actuating the clamp lock switch 124, causing it to pivot about the clamp lock pin 208 (clockwise as shown in

FIGS. 6 and 8). This may allow the closure trigger 120 to return to the open position, causing proximal motion of the closure sleeve and pivoting the anvil 112 proximally and away from the elongate channel 110 of the end effector 104, as described below.

As the closure trigger 120 is moved toward the pistol grip 118, its intermediate section 182 may be pulled proximally, causing the firing trigger 122 to also move proximally to its “firing” position. When in its firing position, the firing trigger 122 may be located at an angle of approximately 45° to the pistol grip 118. To fire the instrument 102, the clinician may first deactivate a firing trigger safety 210. For example, the safety 210 may be pivotally coupled to the closure trigger 120 about a pin 212. A distal portion of the safety 210 may be received into a cavity 214 of the firing trigger 122, preventing the firing trigger 122 from being actuated. The clinician may deactivate the safety 210 by removing it from the cavity 214 and pivoting the safety 210 proximally. This may allow the clinician to actuate the firing trigger 122.

The firing trigger 122 may be biased to an “off” position by a biasing member such as a spring 216 (FIG. 9). When actuated (e.g., against the force of the spring 216), the firing trigger 122 may be rotated clockwise, as shown in FIG. 9. A contactor portion 218 of the trigger may activate a trigger switch 220, e.g., via an actuator 221, which may initiate firing of the instrument 102. Actuation of the trigger switch 220 may activate a motor 222. The motor 222 may be coupled to a gearbox 224 comprising an enclosure 226 and gear cluster 228. The gearbox 224 may gear down the motor 222. In one example embodiment, the motor 222 may rotate at 106,000 RPM, while the gearbox 224 may have a ratio of 509-to-1.

An intermediate gear 230 may be coupled to the output of the gearbox 224. The intermediate gear 230 may be in mechanical communication with a drive gear 232. The drive gear 232 may be rotatable about a drive shaft 234. A biasing member such as a spring 236 may bias the drive gear 232 and/or drive shaft 234 such that the drive gear 232 is in mechanical communication with a geared face 240 of a rack 238. The rack 238 may be coupled to the firing drive member 130 which may, ultimately, be in mechanical communication with the firing bar 108. Accordingly, rotation of the motor 222 may cause rotation of the gearbox 224, leading to rotation of the intermediate 230 and drive 232 gears. Rotation of the drive gear 232 may result in distal or proximal motion of the rack 238, drive member 130, and drive bar 108. Distal and proximal motion of the drive bar 108 may cause the instrument 102 to fire, for example, as described herein below.

When the instrument is fired, the rack 238 may translate distally. A top geared face 242 of the rack 238 may be coupled to a clamp lock 244, causing the clamp lock 244 to translate distally about a pivot pin 246. In its distal position, the clamp lock 244 may contact the clamp switch 124, preventing it from disengaging as described above. In this way, the clinician may be mechanically prevented from releasing the clamp switch 124 while the instrument 102 is in a fired position (e.g., the drive bar 108 is extended distally).

According to various embodiments, the surgical instrument 102 may comprise mechanisms allowing a clinician to disable the motor 222 and manually disengage the firing bar 108. For example, the instrument 102 may comprise an emergency access door 248. The access door 248 may be coupled to a switch, as described below, such that when the clinician opens the access door 248, electric power to the motor 222 may be cut. Below the access door 248, the device 102 may comprise a manual retraction lever 250. The retraction lever 250 may be rotatable about a pivot a pin 252. A locking cam 254 may also be pivotable about the pin 252. After the clini-

cian has opened and/or removed the access door 248, the clinician may pull up on the retraction lever 250. This may cause the lever 250 to rotate about the pin 252 (clockwise as shown in FIG. 9 and counter clockwise as shown in FIG. 6).

Initially, the locking cam 254 may rotate with the retraction lever 250. As the locking cam 254 rotates, a locking arm 256 of the cam 254 may contact a top surface 258 of the drive gear 232, working against the bias of the spring 236 to push the drive gear 232 down and out of contact with the geared face 240 of the rack 238. This may disengage the motor 222 from the rack 238, drive member 130 and drive bar 108. When the locking cam 254 is rotated by a predetermined amount, the locking arm 256 may lock against the drive gear 232, preventing reverse rotation of the locking cam 254.

FIGS. 10-15 illustrate additional details of the operation of the locking cam 254. FIG. 10 illustrates a partial cross-sectional view of one embodiment of the surgical instrument 102 with various components removed for clarity showing the operation of the retraction lever 250. In FIG. 10, the rack 238 is shown in cross-section. FIGS. 11 and 12 illustrate one embodiment of the locking cam 254 during various states of operation. The locking cam 254 may comprise a body portion 260. The locking arm 256 that may pivot, or otherwise flex, with respect to the body portion 260 about a hinge portion 262. The hinge portion 262 may comprise, for example, a living hinge. In one embodiment, the body portion 260 and the locking arm 256 may be unitary and formed from a single piece of material. The locking cam 254 may define a clearance 264 that allows the locking arm 256 to pivot toward the body portion 260. The locking arm 256 may have a tooth 266 that is received by a notch 268 in the body portion 260. On their respective outer peripheries, the body portion 260 may have a first contacting surface 270 and the locking arm 256 may have a second contacting surface 272. In the closed position (FIG. 11), the first contacting surface 270 may be generally aligned with the second contacting surface 272 such that the outer periphery of the locking cam 254 has a generally continuous cammed surface. In the open position (FIG. 12), the locking arm 256 pivots away from the body portion 260 to increase the clearance 264. A gap 258 is created between the first contacting surface 270 and the second contacting surface 272.

Referring now to FIGS. 10, 11, and 12, upon rotation of the lever 250 in the direction indicated by arrow 274, the locking cam 254 is rotated and the second outer surface 272 of the locking arm 256 first contacts a top surface 258 of the intermediate gear 230. As a result of this contact, the locking arm 256 may be pivoted toward the body portion 260 to create a generally continuous periphery. As the locking cam 254 continues to rotate, the second contacting surface 272 and then the first contacting surface 270 exerts force on the intermediate gear 230 to overcome the biasing force applied by the spring 236. As a result, the intermediate gear 230 is pushed in the direction indicated by arrow 275 as the lever 250 is rotated in the direction indicated by arrow 274. The movement of the intermediate gear 230 may decouple it from the geared face 240 of the rack 238 allowing the rack 238 to translate freely. Once the locking arm 256 clears the top surface 258 of the intermediate gear 230, it may pivot to the open position (FIG. 12) to lock the locking cam 254 into place. Once in the open position, the locking cam 254 may be impeded from rotating in the direction indicated by arrow 276 (FIG. 10) due to the engagement of the locking arm 256 with the intermediate gear 230.

FIGS. 13-15 show various embodiments of the locking cam 254 and a intermediate gear 230 during three stages of operation. Various components have been removed and/or

simplified for clarity. As illustrated, the locking cam **254** may be manufactured from a single piece of material. The locking cam **254** comprises a locking arm **256** that is pivotable with respect to a body portion **260**. FIG. 13 shows one embodiment of the locking cam **254** in a non-engaged position. In this position, a distal portion **278** of the locking arm **256** is separated from the body portion **260**. As illustrated in FIG. 14, when the locking cam **254** is rotated in the direction indicated by arrow **274**, the locking arm **256** is drawn toward the body portion **260** to create a generally continuous periphery spanning the locking arm **256** and the body portion **260**. As the locking cam **254** contacts a top face **258** of the intermediate gear **230**, the gear **230** may move in the direction indicated by arrow **280**. As the locking cam **254** continues to rotate in the direction indicated by arrow **274**, eventually the locking arm **256** passes over the drive shaft **234**. As shown in FIG. 15, when the distal portion **278** of the locking arm **256** separates from the body portion **260**, it engages the teeth of the intermediate gear **230** to lock the locking cam **254** into an engaged position. Accordingly, in various embodiments, while the locking cam **254** may be made from a single piece of material, it may function as two parts (e.g., a cam and a locking mechanism).

Referring now to FIG. 6, the retraction lever **250** may also comprise a ratchet arm **282** rotatable about a ratchet pin **284**. As the retraction lever **250** is pulled up, a tooth portion **286** of the ratchet arm **282** may come into contact with the top geared face **242** of the rack **238**. Further rotation of the ratchet lever **250** may cause the tooth **286** to exert a proximally directed force on the rack **238**, causing the drive member **130** and drive bar **108** to translate proximally. Further lifting of the retraction lever **250** may disengage the tooth portion **286** from the top geared face **242**, allowing the clinician to replace the retraction lever **250** towards its original position without causing corresponding distal motion of the rack **238**. Additional proximal motion of the rack **126**, drive member **130** and drive bar **108** may be achieved by additional lifting of the retraction lever **250**, repeating the process described above.

FIG. 17 shows one embodiment of the implement portion **114** of the surgical stapling and severing instrument **102** in disassembled form. The staple cartridge **132** is shown as being comprised of a cartridge body **304**, a wedge sled **306**, single and double drivers **308**, staples **310**, and a cartridge tray **312**. When assembled, the cartridge tray **312** holds the wedge sled **306**, single and double drivers **308**, and staples **310** inside the cartridge body **304**.

The elongate channel **110** may have a proximally placed attachment cavity **314** that receives a channel anchoring member **316** on the distal end of the frame **126** for attaching the end effector **104** to the handle portion **106**. The elongate channel **110** may also have an anvil cam slot **316** that pivotally receives an anvil pivot **318** of the anvil **112**. The closure sleeve **128** that encompasses the frame **126** may include a distally presented tab **320** that engages an anvil feature **324** proximate but distal to the anvil pivot **318** on the anvil **112** to thereby effect opening and closing of the anvil **112**. The firing drive member **130** is shown as being assembled from the firing bar **108** attached to a firing connector **326** by pins **328**, which in turn is rotatably and proximally attached to the metal drive rod **330**. The firing bar **108** is guided at a distal end of the frame by a slotted guide **332** inserted therein.

With particular reference to FIG. 18, a portion of the staple cartridge **132** is removed to expose portions of the elongate channel **110**, such as recesses **300**, **302** and to expose some components of the staple cartridge **132** in their unfired position. In particular, the cartridge body **304** (shown in FIG. 17) has been removed. The wedge sled **306** is shown at its proximal,

unfired position with a pusher block **334** contacting the middle pin **144** (not shown in FIG. 18) of the firing bar **108**. The wedge sled **306** is in longitudinal sliding contact upon the cartridge tray **312** and includes wedges **308** that force upward the single and double drivers **308** as the wedge sled **306** moves distally. Staples **310** (not shown in FIG. 18) resting upon the drivers **308** are thus also forced upward into contact with the anvil forming pockets **290** on the anvil **112** to form closed staples. Also depicted is the channel slot **142** in the elongate channel **110** that is aligned with the vertical slot **154** in the staple cartridge **132**.

FIG. 19 depicts the end effector **104** of FIG. 18 with all of the staple cartridge **132** removed to show the middle pin **144** of the firing bar **108** as well as portion of the elongate channel **110** removed adjacent to the channel slot **142** to expose the firing bar cap **140**. In addition, portions of the shaft **116** are removed to expose a proximal portion of the firing bar **108**. Projecting downward from the anvil **112** near the pivot, a pair of opposing tissue stops **346** may prevent tissue being positioned too far up into the end effector **104** during clamping.

FIG. 20 depicts one embodiment of the end effector **104** closed in a tissue clamping position with the firing bar **108** unfired. The upper pin **134** is shown in the anvil pocket **136**, vertically aligned with the anvil slot **138** for distal longitudinal movement of the firing bar **108** during firing. The middle pin **144** may be positioned to push the wedge sled **306** distally so that wedge **308** sequentially contacts and lifts double drivers **308** and the respective staples **310** into forming contact with staple forming pockets **290** in the lower surface **288** of the anvil **112**. According to various embodiments, the end effector **104** may implement a mechanical lock-out mechanism. The mechanical lock-out mechanism may prevent the instrument **102** from being fired twice without reloading a new staple cartridge **132**. For example, it will be appreciated that firing the instrument **102** without a loaded staple cartridge present may cause tissue to be cut, but not fastened. The lock-out may be implemented in any suitable manner. For example, the firing bar **108**, upon retraction in the proximal direction, may be shifted by the elongate channel **110**, or other component, such that the upper pin **134** is no longer in alignment with the anvil slot **138**, preventing the firing bar **108** from moving distally (e.g., re-firing). Installation of a new staple cartridge **132** to the elongate channel **110** may snap the firing bar **108** back, aligning the upper pin **134** with the anvil slot **138** and allowing re-firing. It will be appreciated that any suitable mechanism in the end effector or the handle **106** may be utilized to implement a mechanical lock-out.

FIG. 21 depicts one embodiment of the upper surface **294** of the staple cartridge **132** with the firing bar **108** in its unfired, proximal position. The stapler apertures **292** are arrayed on each side of the vertical slot **154** in the staple cartridge **132**. FIG. 22 depicts one embodiment of the end effector **104** near the pivot showing that the elongate channel **110** has opposing ramp portions **348** to thereby cooperate with the tissue stops **346** of the anvil **112** to prevent tissue from jamming the end effector **104**. Also depicted in greater detail are the double drivers **308** and their relation to the staples **310**.

FIGS. 24-26 illustrate one embodiment of the end effector **104** at various stages of firing. In use, the surgical stapling and severing instrument **102** may be used to cut and staple tissue. In FIGS. 1-2, the instrument **102** is shown in its start position, having had an unfired, fully loaded staple cartridge **132** snap-fitted into the distal end of the elongate channel **110**. Both triggers **120**, **122** are forward and the end effector **104** is open, such as would be typical after inserting the end effector **104** through a trocar or other opening into a body cavity. The instrument **102** may then be manipulated by the clinician such

11

that tissue **340** to be stapled and severed is positioned between the staple cartridge **132** and the anvil **112**. FIG. **23** illustrates the end effector **104**, according to one embodiment, with tissue **340** present between the staple cartridge **132** and the anvil **112**.

Next, the clinician moves the closure trigger **120** proximally until positioned directly adjacent to the pistol grip **118**, locking the handle portion **106** into the closed and clamped position. The retracted firing bar **108**, shown in FIG. **24** in the end effector **104** may not impede the selective opening and closing of the end effector **104**, but rather may reside within the anvil pocket **136**. With the anvil **112** closed and clamped, the firing bar **108** may be aligned for firing through the end effector **104**. In particular, the upper pin **134** may be aligned with the anvil slot **138** and the elongate channel **110** may be affirmatively engaged about the channel slot **142** by the middle pin **144** and the firing bar cap **140**.

After tissue clamping has occurred, the clinician may move the firing trigger **122** proximally causing the firing bar **108** to move distally into the end effector **104**, shown in FIG. **25**. In particular, the middle pin **144** enters the staple cartridge **132** through the firing drive slot **146** to cause the firing of the staples **310** via wedge sled **306** toward the anvil **112**. The lower most pin, or firing bar cap **140**, cooperates with the middle pin **144** to slidably position cutting edge **152** of the firing bar **108** to sever tissue. The two pins **140**, **144** also position the upper pin **134** of the firing bar **108** within longitudinal anvil slot **138** of the anvil **112**, affirmatively maintaining the spacing between the anvil **112** and the elongate channel **110** throughout its distal firing movement.

The clinician may continue moving the firing trigger **122** until brought proximal to the closure trigger **120** and pistol grip **118**. Thereby, all of the ends of the staples **310** may be bent over as a result of their engagement with the anvil **112**, as shown in FIG. **26**. The firing bar cap **140** may be arrested against a firing bar stop **342** projecting toward the distal end of the channel slot **142**. The cutting edge **152** may have traversed completely through the tissue. The process is complete by releasing the firing trigger **122**. Releasing the firing trigger **122** may, as described herein below, cause the motor **222** to reverse its rotation, causing retraction of the firing bar **108**. Upon retraction of the firing bar **108**, the clinician may depress the clamp switch **124**. (e.g., while simultaneously squeezing the closure trigger **120**) This may open the end effector **104**.

Referring back to FIG. **1**, the handle **106** of the instrument **102** may house at least one battery unit **506**. The battery unit **506** may comprise a single battery or a plurality of batteries arranged in a series and/or parallel configuration. The handle **502** may comprise a battery dock **508** to which the battery unit **506** may be attached. The battery dock **508** may be any suitable structure for coupling the battery unit **506** to the instrument **102**. For example, the battery dock **508** may be or comprise a cavity in the handle **106** configured to receive at least a portion of the battery unit **506**, as illustrated. In other embodiments, the battery dock **508** may be implemented using a variety of other structures. In one embodiment, the battery dock **508** may comprise a post that is received by the battery unit **506**. In one embodiment, the pistol grip **120** may comprise the battery dock **508**. In any event, as discussed in more detail below, the battery dock **508** may comprise a protruding portion to interact with the battery unit **506** upon attachment of the battery unit **506** to the handle **502**. Once attached, the battery unit **506** may be electrically connected to and may provide power to the motor **222** of the instrument **102**.

12

FIGS. **27-29** schematically illustrate one embodiment of the battery unit **506** and a portion of the instrument **102** showing the attachment and detachment of the battery unit **506** to the instrument **102**. The battery unit **506** may comprise a drain **512** that automatically completes a circuit within the battery unit **506** upon attachment to the instrument **102**. The drain may serve to slowly reduce the charge of the battery unit **506** over time. Once the battery unit **506** has been sufficiently drained it may be disposed as non-hazardous waste, for example. The battery unit **506** may comprise a voltage source **510**. In one embodiment, the voltage source **510** is a lithium battery and comprises at least one cell selected from the group consisting of a CR123 cell and a CR2 cell. As is to be appreciated, any suitable voltage source may be used. The battery unit **506** may also comprise a drain **512** that may be electrically coupled to the voltage source **510** when a switch **516** is closed. The battery unit **506** and the instrument **102** each comprise electrically conductive contacts **518**, **520**, respectively, that are placed into contact upon attachment of the battery unit **506** to the instrument **102**. FIG. **27** illustrates the battery in a non-attached position. The switch **516** is in an open position and the voltage source **510** may be in a fully charged condition. FIG. **28** illustrates that battery unit **506** in an attached position. The conductive contacts **518** of the battery unit **506** are in electrical communication with the contacts **520** of the instrument thereby allowing the battery unit **506** to supply energy to the circuit **514** (FIG. **46**). In the attached position, the switch **516** may transition to the closed position to electrically couple the voltage source **510** to the drain **512**. Energy will flow from the voltage source **510** through the drain **512** during operation of the instrument. In other words, the drain **512** will be draining the charge from the voltage source **510** concurrently as the battery unit **506** is supplying operational power to the instrument **102**. As discussed in more detail below, a portion of the instrument **102** may physically interact with the drain **512** during attachment of the battery unit **506** to the instrument **102** to transition the switch **516** from the open to the closed state. FIG. **29** illustrates the battery unit **506** in a non-attached position. In one embodiment, the switch **516** remains in the closed position to continue to drain the voltage source **510** even after the battery unit **506** has been detached from the instrument **102**.

FIG. **30** illustrates a graph **600** of the voltage level of one embodiment of the battery unit **506** over time, as measured from the time of attachment to the instrument **102**. The graph **600** includes three example discharge curves **602**, **604**, **606**. As illustrated by the first discharge curve **602**, the voltage of the power source **510** may drop below 2.0 volts after around 28 hours. As illustrated by the second discharge curve **604**, the voltage of the power source **510** may drop below 2.0 volts after around 30 hours. As illustrated by the third discharge curve **606**, the voltage of the power source **510** may drop below 2.0 volts after around 33 hours. The overall shape of the discharge curve may depend upon, for example, the level of activity of the instrument **102** during the surgical procedure. For example, the instrument associated with the first discharge curve **602** was more heavily used during the surgical procedure than the instrument associated with discharge curve **606**. In any event, the drain **512** may maintain the voltage level of the battery unit **506** at a satisfactory level for a certain time period to ensure that the instrument can be used for its intended purpose during the course of the surgical procedure. For example, in one embodiment, the voltage level of the battery unit **506** may be maintained around 6 volts for approximately 12 hours. After 12 hours, the voltage level gradually decreases to a non-hazardous level. As is to be

13

appreciated, the drain **512** may be calibrated to deplete the voltage source faster or slower.

In one embodiment, a resistive element may be used to reduce the energy level of the voltage source. FIG. **31** shows a simplified circuit diagram of one embodiment of a battery unit **616** comprising a drain **612**. The battery unit **616** may be attached to an instrument **102**, for example, via its contacts **618**. In this embodiment, the battery unit **616** may comprise a first grouping of cells **610** and a second grouping of cells **611**. In one embodiment, the first and second grouping of cells **610**, **611** may be lithium batteries. The first and second grouping of cells **610**, **611** may each have a plurality of separate cells **610a**, **610b**, **611a**, **611b** arranged in a parallel formation. For example, the first and second grouping of cells **610**, **611** may each be 6 VDC and arranged in a series configuration to produce 12 VDC at the contacts **618** of the battery unit **616** when fully charged. The cells **610a**, **610b**, **611a**, **611b**, however, may be electrically connected to one another in series or parallel or any other combination thereof. The number of cells **610a**, **610b**, **611a**, **611b** may be chosen to reduce the fire hazard resulting from the battery unit **616**. For example, the number of connected cells may be selected such that the cumulative energy available to an arc or short is less than the energy required to ignite common shipping and/or packing materials. According to various embodiments, this value may be defined by appropriate government regulations.

In one embodiment, the drain **612** may comprise a first resistive element **622** and a second resistive element **624**. As is to be appreciated, in some embodiments, the battery unit **616** may comprise, for example, multiple drains **612** each having more or less than two resistive elements or other circuitry. In the illustrated embodiment, the first resistive element **622** is coupled across a first anode **626** and a first cathode **628** of the first grouping of cells **610** through a first switch **630**. The first resistive element **624** may be coupled across a second anode **632** and a second cathode **634** of the second grouping of cells **611** through a second switch **636**. The first and second switches **630**, **636** may be closed upon attachment of the battery unit **616** to the surgical instrument **102** in order to initiate the draining of the first and second grouping of cells **610**, **611**.

The value of the resistive elements utilized by the drain **612** may vary based on implementation. In one embodiment, the first resistive element **622** has a resistance in the range of about 90 ohms to about 110 ohms. In one embodiment, the first resistive element **622** has a resistance in the range of about 97 ohms to about 104 ohms. In one embodiment, the resistive element **622** is 102.9 ohms and has a power rating of 1 watt. The determination of the necessary resistance is based at least partially on the capacity of the voltage source, the voltage level of the voltage source, and the desired temporal length of the drainage curve. For example, in one embodiment the battery capacity of the first grouping of cells **610** is 1400 mAh, the voltage level is 6 VDC, and the target drain time is 24 hours. Dividing 1400 mAh by 24 hours yields a current of 0.0582 A. Using Ohm's law, 6 V divided by 0.582 A yields a resistance of 102.9 ohms. With a current of 0.583 A and a resistance of 102.9 ohms, the power dissipated by the resistor is 350 W. As is to be appreciated, different voltage levels, battery capacities, and desired time of discharge will result in different resistance values.

FIG. **32** is a simplified circuit diagram of one embodiment of a battery unit **716** comprising a first drain **712** and a second drain **713**. The battery unit **716** may be attached to an instrument **102**, for example, via its contacts **718**. In this embodiment, the battery unit **716** comprises a first grouping of cells **710**, a second grouping of cells **711**, and a third cell **714**. The

14

first drain **712** comprises a first resistive element **722** and a second resistive element **724**. The second drain **713** comprises a third resistive element **726**. The resistive elements **722**, **724**, **726** are coupled to respective cells through switches **730**, **736**, and **738**. The switches **730**, **736**, and **738** may be closed upon attachment of the battery unit **716** to the surgical instrument **102** in order to initiate the draining of the first and second grouping of cells **610**, **611** and the third cell **716**. The resistance of the third resistive element **726** may be similar or different from the resistances of the first and second resistive element **722**, **724**. As described above, the resistance of the third resistive element **726** may at least partially depend on the voltage of the third cell **714** and the desired characteristics of the drainage curve.

FIGS. **33-36** are perspective views of one embodiment of a battery unit **506** implementing the schematic of the battery unit **616** shown in FIG. **31**. The battery unit **506** may comprise a casing **802** defining an interior cavity **810**. While the interior cavity **810** is illustrated in a central portion of the casing **802**, it is to be appreciated that the internal cavity **810** may be positioned in any suitable location. The casing **802** may be covered by a cap **804** that may be secured to the casing **802** utilizing one or more mechanical latches **806**, **808**. FIG. **34** illustrates one embodiment of the battery unit **506** with the cap **804** removed to show a plurality of cells **812** within. Any suitable number and/or type of cells **812** may be used. For example, CR123 and/or CR2 cells may be used. FIG. **35** illustrates one embodiment of the battery unit **506** with a portion of the casing **802** removed to reveal the cells **812**. FIG. **36** illustrates one embodiment of the battery unit, with a portion of the casing **802** missing as in FIG. **35**. FIG. **36** shows the battery pack **506** from a side **890** positioned to face distally when the battery pack **506** is installed on the surgical device **102**. The interior cavity **810** is visible as well as a pair of contacts **886**, **888** in electrical communication with the various cells **812**.

FIGS. **37** and **38** illustrate cross-sectional views of one embodiment of the battery unit **506** including a translatable drain **812**. The drain **812** may be positioned within the interior cavity **810** and may be translatable within the interior cavity **810** in the directions of arrow **815**. FIG. **37** shows the drain **812** in an open position and FIG. **38** shows the drain **812** in a closed position. The drain **812** may comprise at least two contacts **816**, **818**. When the drain **812** is in the open position, a portion of the contacts **816**, **818** may touch a non-conductive portion of the casing **802**, such as fingers **820**, **822**. According to various embodiments, the contacts **816**, **818** may be biased to exert a force against the fingers **820**, **822** in order to resist movement of the drain **812** in the direction of the arrows **815**. Also, in some embodiments, the fingers **820**, **822** may define one or more protrusions or stepped down portions, as shown in FIGS. **37** and **38**. The battery unit **506** may also comprise one or more electrodes, such as first electrode **824** and second electrode **826**. The first and second electrodes **824** and **826** may each be electrically coupled to a cathode or an anode of cells contained within the battery unit **506**. In the closed position (FIG. **38**), the contacts **816**, **818** are in electrical connection with the electrodes **824**, **826**, thereby allowing the voltage source to discharge through the drain **812**. As discussed in more detail below, the drain **812** may be translated from the open position to the closed position upon attachment of the battery unit **506** to a surgical instrument.

FIG. **43** is a perspective view of one embodiment of the drain **812** in accordance with one non-limiting embodiment. The contacts **816**, **818** of the drain **812** may be coupled to a base portion **830** of the drain **812**. Similarly contacts **836**, **838** of the drain **812** may be coupled to the base portion **830** of the

15

drain **812**. According to various embodiments, the contacts **816**, **818** may be electrically connected to one another via a resistive element (not shown) mounted to a circuit board **832**. Similarly, the contacts **836**, **838** may be electrically connected to one another via a resistive element mounted to the circuit board **832**. As illustrated, the contacts **816**, **818**, **836**, **838** may have a bend or curvature to bias the contacts towards an outward position when they are inwardly compressed. Additionally, in one embodiment, the distal end of each of the contacts **816**, **818**, **836**, **838** may have an inwardly turned section. The base portion **830** may comprise a contacting surface **840** that engages the instrument when the battery unit **506** is attached to the instrument. Through this engagement, the drain **812** may be translated relative to the casing **802**.

FIGS. **39-42** illustrate multiple views of a one embodiment of a battery dock **850**. The battery dock **850** may be positioned within the handle **106** of the instrument **102** and may receive the battery unit **506**. For example, the battery dock **850** may comprise a protruding member or bulkhead **858**. The battery dock **850** may be positioned within the base sections **156**, **158** and, in some embodiments, may be coupled to the frame sections **160**, **162** such that the protruding member **858** extends proximally. The battery unit **506** may be installed into the device **102** by pushing it distally against the battery dock **850**. The protruding member **858** of the battery dock **850** may extend into the exterior cavity **810** of the battery unit **506**. Contacts **882**, **884** of the battery dock **850** may also extend into the interior cavity **810** of the battery unit **506**. Within the cavity, the contacts **882**, **884** of the battery dock **850** may be in electrical communication with the contact **886**, **888** of the battery unit **506** (FIG. **36**). When the contacts **886**, **888** of the battery unit **506** come into contact with the contacts **882**, **884** of the battery dock **850**, the battery unit **506** may be in electrical communication with the instrument **102**.

FIG. **44** illustrates one embodiment of the battery unit **506** attached to the battery dock **850**. For clarity, various components have been removed. Referring now to FIGS. **37**, **38**, **43** and **44** as well as to FIGS. **39-42**, the battery dock **850** is shown with its protruding member **858** sized to be received by the cavity **810** (FIG. **33**) of the battery unit **506**. Prior to attachment, the drain **812** may be in the open position (FIG. **37**). During attachment of the battery unit **506** to the battery dock **850**, the protruding member **858** is inserted into the cavity **810** and the battery unit **506** is moved relative to the battery dock **850** in the direction indicated by arrow **862**. Eventually the distal end **860** of the protruding member **858** contacts the contacting surface **840** of the drain **812**. As the user continues to attach the battery unit **506**, the drain **812** is translated relative to the casing **802** in the direction indicated by arrow **864** and moves into the closed position (FIG. **38**). In this position, the battery unit **506** commences to slowly drain. When the battery unit **506** is removed from the battery dock **850**, the drain **812** may remain in the position shown in FIG. **38**. In this way, the cells (not shown) of the battery unit **506** may drain any remaining charge across a resistive element either before or during disposal.

As is to be appreciated, the translatable discharge drain of the battery unit is not limited to the implementation illustrated in FIG. **44**. FIGS. **45** and **46**, for example, illustrate one embodiment of a battery unit **900** and drain **912** with various components removed for clarity. The drain **912** that is translatable between an open position (FIG. **45**) and a closed position (FIG. **46**). In the open position, contacts **916**, **918** are engaged with non-conductive portions of a casing **920**, **922**, respectively. The drain **912** may ride in a track **914** when translating between the open position and the closed position. FIG. **46** shows the battery unit **900** in a closed position after a

16

ram **958** has translated the drain **912** in the direction indicated by arrow **964**. The ram **958** may be a component of a battery dock of a surgical instrument, for example. In one embodiment, the battery dock comprises a cavity that is dimensioned to receive the battery unit **900**, and the ram **958** is positioned within the cavity. In the closed position, the contacts **916**, **918** are in electrical contact with electrodes **924**, **926**. The drain **912** may comprise a printed circuit board **932** to which at least one resistive element is mounted using a surface mount or a through-hole connection, for example.

FIGS. **47** and **48** illustrate a battery unit **1000** in accordance with another non-limiting embodiment. Various components have been omitted for clarity. The battery unit **1000** may comprise a drain **1012** that may be translatable between an open position (FIG. **47**) and a closed position (FIG. **48**). The battery unit **1000** may also comprise a first electrode **1024** with a contact **1025** and a second electrode **1026** with a contact **1027**. The electrodes **1024**, **1026** may be in contact with cells (not shown) of the battery unit **1000**. In the open position, contacts **1016**, **1018** of the drain **1012** are not engaged with contacts **1025**, **1027** of the electrodes **1024**, **1026**. The drain **1012** may ride in a track **1014** when translating between the open position and the closed position. FIG. **48** shows the battery unit **1000** in a closed position after a ram **1058** has translated the drain **1012** in the direction indicated by arrow **1064**. The ram **1058** may be a component of a battery dock of a surgical instrument, for example. In the closed position, the contacts **1016**, **1018** of the drain **1012** are in electrical contact with the contacts **1025**, **1027** of the electrodes **1024**, **1026**. The drain **1012** may comprise a printed circuit board **1032** that includes at least one resistive element. In some embodiments, the contacts **1016**, **1018** themselves may comprise the resistive elements. In fact, the resistive elements may be elements of any suitable resistance value and any suitable mechanical configuration.

FIG. **49** is a perspective view of one embodiment of a battery unit **1100**. FIGS. **50** and **51** show internal views of the battery unit **1100** during various stages of operation with various components removed for clarity. The battery unit **1100** has one cell **1102** and an outer casing **1104** that defines a cavity **1110**. The outer casing **1104** may be non-conductive and have conductive contacts for supplying energy to circuitry of a surgical instrument when the battery unit **1100** is attached to a surgical instrument. In one embodiment, the battery unit **1100** is received by a cavity in a pistol grip portion of a surgical instrument. The battery unit **1100** comprises a drain **1112** that is translatable between an open position (FIG. **50**) and a closed position (FIG. **51**). In one embodiment the drain **1112** has first and second contacts **1116**, **1118** that are coupled to a circuit board **1132**. The circuit board **1132** may include, for example, at least one resistive element. In some embodiments, the circuit board **1132** includes additional circuitry. The battery unit **1100** comprises a first electrode **1124** coupled to an anode of the cell **1102** and a second electrode coupled to a cathode of the cell **1102**. Before the battery unit **1100** is attached to an instrument, the drain **1112** is in the open position (FIG. **50**). In the illustrated embodiment, the first contact **1116** is electrically coupled to the first electrode **1124** and the second contact **1118** is resting on, or otherwise contacting, a non-conductive finger **1120**. As the battery unit **1100** is attached to an instrument, a protruding portion **1158** of the instrument may be received by the cavity **1110** and contact the drain **1112** to drive the drain **1112** in the direction indicated by the arrow **1164**. In the closed position (FIG. **51**) the first contact **1116** is electrically coupled to the first electrode **1124** and the second contact **1118** is electrically coupled to the second electrode **1126**. In this position, a

17

closed circuit is created that allows the cell 1102 to discharge energy through the drain 1112. Additional embodiments of battery units are disclosed in commonly owned U.S. patent application Ser. No. 12/884,995 entitled, "POWER CONTROL ARRANGEMENTS FOR SURGICAL INSTRUMENTS AND BATTERIES," filed on Sep. 17, 2010 and incorporated herein by reference in its entirety. Still other embodiments of battery units are disclosed in commonly owned U.S. patent application Ser. No. 12/884,838, entitled "SURGICAL INSTRUMENTS AND BATTERIES FOR SURGICAL INSTRUMENTS," filed on Sep. 17, 2010 and also incorporated herein by reference in its entirety.

According to various embodiments, electrical connection of the battery unit 506 or other power supply to the motor 222 may initiate a firing of the instrument 102. FIG. 52 illustrates one embodiment of a control circuit 1200 that may control a connection between the battery unit 506 or other power supply and the motor 222 or other drive device for firing the instrument 102. According to various embodiments, the control circuit 1200 may be implemented with components on a PC board 1202 shown in FIG. 7. The control circuit 1200 may comprise various switches and other components for controlling the connection between the battery unit 506 and the motor 222. The battery unit 506 is shown with a positive electrode 1212 and a negative electrode 1210. Similarly, the motor 222 is shown with a positive terminal 1216 and a negative terminal 1214. It will be appreciated that the polarity of the circuit 1200 could be reversed, for example, based on other design considerations.

The control circuit 1200 may comprise a firing switch 220 (also shown in FIG. 9), which may be in mechanical communication with the firing trigger 120 (e.g., via an actuator 221). The control circuit 1200 may also comprise an end-of-stroke/reverse motor switch 1204 and a clamp switch 1206. The end-of-stroke/reverse motor switch 1204 may be actuated when the firing bar 108 reaches the end of its stroke (e.g., at or near its distal-most position). Also, according to various embodiments, the end-of-stroke/reverse motor switch 1204 may be actuated manually by the clinician prior to the end of the stroke of the firing bar 108 to abort and/or reverse the firing of the instrument 102. A clamp switch 1206 may be actuated when the end effector 104 is closed (e.g., the anvil 112 and elongate channel 110 are brought into contact with one another) and also when the end effector 104 is opened. A clamping relay 1208 may also be a component of the circuit 1200. According to various embodiments, the relay 1208 may be a non-solid state relay (e.g., a mechanical relay, an electromagnetic relay, etc.). This may allow the instrument 102 to be subjected to gamma sterilization as well as other sterilization techniques that have the potential to damage solid state components. It will be appreciated, however, that the clamping relay 1208 may, in various embodiments, be replaced with any sort of switching device including, for example, a field effect transistor (FET), bipolar junction transistor (BJT), etc. Also, in some embodiments, the relay 1208 may be replaced with a microprocessor.

When the instrument is ready for use (e.g., a staple cartridge 132 is loaded to the elongate channel 110), the control circuit 1200 may be configured as shown in FIG. 52. The end-of-stroke/reverse motor switch 1204 may be connected between 1 and 3, creating an electrical connection between the positive electrode 1212 of the battery and the positive terminal 1216 of the motor 222. The relay 1208 may be in a closed state. For example, an electrical connection may be made between pins 4 and 5 of the relay 1208. The firing switch 220 may be connected between points 1 and 3, creating an electrical connection between the positive electrode

18

1212 of the battery 506 and the negative terminal 1214 of the motor 222. Because both terminals 1214, 1216 of the motor 222 are connected to a single electrode 1212 of the battery 506, the motor 222 may not operate.

The clinician may initiate a firing operation by actuating the firing trigger 122, which, via the actuator 221, may cause the firing switch 220 to transition to a second state where the points 1 and 3 are connected. This may create an electrical connection between the negative terminal 1214 of the motor 222 and the negative electrode 1210 of the battery 506 (e.g., via pins 1 and 2 of the firing switch 220 and pins 4 and 5 of the relay 1208). This may cause the motor 222 to rotate in a forward direction. For example, the motor may rotate the gearbox 224, intermediate gear 230, drive gear 232 and rack 238 to ultimately push the firing bar 108 distally.

When the firing bar 108 reaches the end of its stroke, the end-of-stroke switch 1204 may transition from the position shown in FIG. 52 to a position where the points 1 and 2 of the switch 1204 are connected. This may connect pin 3 of the relay 1208 to the negative electrode 1210 of the battery 506 (e.g., via the pin 4-5 connection of the relay 1208). In turn, this may energize the relay 1208 causing removal of the electrical connection between pins 4 and 5 and generation of an electrical connection between pins 5 and 6. When the clinician releases the firing trigger 122, the firing switch may revert to the state shown in FIG. 52. This may cause the motor 222 to be connected to the battery 506 with a reverse polarity. For example, the positive terminal 1216 of the motor 222 may be connected to the negative electrode 1210 of the battery 506 via the switch 1204 and the relay 1208 (e.g., via pins 5 and 6). The negative terminal 1214 of the motor 222 may be connected to the positive electrode 1212 of the battery 506 via the firing switch 220. As a result, the motor 222 may rotate in reverse, pulling the firing bar 108 proximally, via the gearbox 224, intermediate gear 230, drive gear 232 and rack 238.

At the conclusion of the firing operation, the relay 1208 may be in a state where there is no electrical connection between pins 4 and 5. In this state, the instrument 102 may not be re-fired (e.g., the motor 222 may not be connected to the battery 506 with the correct polarity to cause forward rotation). According to various embodiments, a clamp switch 1206 may be positioned to energize the relay 1208 (e.g., pulling pin 1 low) in order to transition the relay 1208 back to the initial state having an electrical connection between pins 4 and 5. This may allow the instrument 102 to fire again. The clamp switch 1206 may be in mechanical communication with a portion of the drive train actuated by the closure trigger 120 to close the anvil 114 against the elongate channel 110. For example, the clamp switch 1206 may be in mechanical communication with the clamp lock 244 described herein above. When the anvil 114 is closed against the elongate channel 110 (e.g., when the clamp lock 244 is engaged), the switch 1206 may be in the position shown in FIG. 52, resulting in an electrical connection between points 1 and 3 of the switch 1206. When the clamp lock 244 is disengaged, the clamp switch 1206 may be configured to create an electrical connection between points 1 and 2, energizing the relay 1208 as described. Accordingly, after the instrument 102 is fired, the circuit 1200 may be configured to prevent the motor 222 from operating in the forward direction until the end effector 104 is re-opened. This may prevent the clinician from accidentally re-firing the instrument 102 before the end effector 104 is opened to install a new staple cartridge 132. According to various embodiments, the instrument 102 may comprise a mechanical lock-out device in addition to the relay lock-out implemented by the circuit 1200. The circuit 1200, as described herein, however, may prevent the clinician from

driving the instrument 102 into the mechanical lock-out. This may save wear and tear on the instrument 102 and may also prevent clinician confusion that may occur when the device is in a mechanical lock-out state.

FIG. 53 illustrates one embodiment of the control circuit 1200 with additional switches and features. For example, the circuit 1200, as shown in FIG. 53, may additionally comprise an emergency access or bailout door switch 1218. The emergency access door switch 1218 may be in mechanical communication with the emergency access door 248. For example, when the emergency access door 248 is in place, the switch 1204 may be closed, as shown in FIG. 53. When the emergency access door 248 is removed, the switch 1204 may be opened, creating an open circuit relative to the negative terminal of the battery 506. A stroke position switch 1220 may be connected to switch a resistive element 1222 into and out of the circuit 1200 based on the position of the firing bar 108. The resistive element may be a single resistor and/or a resistor network connected in series, parallel (as shown) or any other suitable configuration. When the resistive element 1222 is switched into the circuit 1200, the current provided to the motor 222 may be reduced. This may reduce the speed and torque provided by the motor 222. Additionally, the control circuit 1200, as illustrated in FIG. 53 may comprise a PTC or other thermal fuse element 1224 to break a connection between the motor 222 and the battery 506 in the event that too much heat is generated (e.g., by the resistive element 1222).

FIG. 54 is a flowchart showing one embodiment of a process flow 1301 showing the firing of the instrument 102 utilizing the control circuit 1200 as illustrated in FIG. 53. At 1300, the instrument 102 may be ready to fire. For example, the switches 1218, 1206, 1220, 220, 1204 and relay 1208 may be configured as illustrated in Table 1 below:

TABLE 1

Switch	Pin/Point Connection
Emergency Access Door (1218)	1-2
Clamp (1206)	1-2
Stroke Position (1220)	1-2
Fire (220)	1-3
End-of-stroke/Motor Direction (1204)	1-3
Relay (1208)	4-5

At 1302, the clinician may actuate the firing trigger 122. This may cause the fire switch 220 to close, creating a connection between points 1 and 2 of the switch 220. Accordingly, the positive terminal of the motor 222 may be connected to the positive electrode 1212 of the battery 506 via the end-of-stroke/motor direction switch 1204. The negative terminal 1214 of the motor 222 may be connected to the negative electrode 1210 of the battery 506 via the thermal fuse element 1224, the resistive element 1222, and the connection between pins 4 and 5 of the relay. This may cause rotation of the motor 222 resulting in distal movement of the firing bar 108 (e.g., via the gearbox 224, intermediate gear 230, drive gear 232 and rack 238). Because the resistive element 1222 is electrically connected between the motor 222 and the battery 506, the current provided to the motor 222 may be reduced. This may, in turn, reduce the speed and/or torque provided by the motor 222 while the resistive element 1222 is active.

At 1304, the firing bar 108 may pass a predetermined position in its firing stroke. This may cause the stroke position switch 1220 to be opened, causing a connection between

points 1 and 2 of the switch 1220. This may, in turn, switch the resistive element 1222, thermal fuse 1224, and relay 1208 out of circuit, allowing full current to be provided to the motor 222. The predetermined position in the firing stroke, in various embodiments, may be a point past which a mechanical lock-out is no longer possible and/or likely. For example, the resistive element 1222 may be utilized to limit the current to the motor 222 during the portion of the firing stroke where the firing bar 108 or other drive train element may encounter a mechanical lock-out. This may limit damage to the drive train or other component of the device 102 if the mechanical lock-out is encountered. When the possibility of encountering a mechanical lock-out has passed, the stroke position switch 1220 may be actuated to switch out the resistive element 1222, allowing full power to be provided to the motor 222 (e.g., for cutting tissue).

The firing bar 108 may reach the end of its stroke (e.g., at or near its distal-most position) at 1306. At this point, the end-of-stroke/motor direction switch 1204 may be actuated, causing it to be connected between points 1 and 2. In this way, the positive terminal 1216 of the motor 222 may be electrically connected to the negative electrode 1210 of the battery 506. The pin 3 of the relay 1208 may also be electrically connected to the negative electrode 1210 of the battery 506, energizing the relay 1208 and breaking the connection between relay pins 4 and 5. When the clinician releases the trigger 122 at 1308, the firing switch 220 may also be actuated, causing it to be connected between points 1 and 2. This may cause the negative terminal 1214 of the motor to be electrically connected to the positive electrode 1212 of the battery 506. In this way, the rotation direction of the motor 222 may be reversed, causing the motor 222 to return the firing bar to its initial, proximal position (e.g., via the gearbox 224, drive gear 232 and rack 238).

Similar to embodiment described above, when the relay 1208 is opened (e.g., the connection between pins 4 and 5 is broken), it may not be possible to rotate the motor 222 in a forward direction to fire the firing bar 108 until the clamp switch 1206 is actuated (e.g., by opening the end effector 104). In this way, the clinician may be prevented from re-firing the instrument 102 prior to opening the end effector 104, for example, to load a new staple cartridge 132. Also, similar to the embodiment described above, the clinician may abort a firing stroke by manually switching the end-of-stroke/motor direction switch 1204 to the state where points 1 and 2 are connected, causing the circuit 1200 and instrument 102 to behave as described above with respect to 1306 and 1308.

FIGS. 55-59 show the orientation and operation of various embodiments of the switches 1218, 1206, 1220, 220, and 1204 described above. FIG. 55 illustrates a perspective view of one embodiment of the circuit board 1202 coupled to the battery dock 850. The circuit board 1202 and battery dock 850, as shown, may be positioned within the handle 106 of the instrument 102, for example, as illustrated in FIG. 7. FIG. 55 shows, on the circuit board 1202, the emergency access door switch 1218, the clamp switch 1206, the stroke position switch 1220, the trigger switch 220 and the end-of-stroke/motor direction switch 1204. FIG. 56 illustrates a cut away view of one embodiment of the instrument 102 showing the emergency access door switch 1218. The switch 1218 may comprise an actuator 1304, which may be spring biased. The emergency access door 248, as shown, may comprise an arm 1302. The arm 1302 may be positioned under the actuator 1304 of the switch 1218. When the emergency access door 248 is removed, the arm 1302 may be removed from under the actuator 1304, changing the state of the switch 1218.

21

FIG. 57 illustrates another cut away view of one embodiment of the instrument 102 showing the clamp switch 1206. The clamp switch 1206 may comprise an actuator 1306. The actuator 1306 may be positioned such that the state of the switch 1206 is changed when the clamp release button 124 is actuated to unclamp the end effector 104.

FIG. 58 shows another cut away view of one embodiment of the instrument 102 showing the stroke position switch 1220. The stroke position switch 1220 may comprise an actuator 1308 and an actuator lever 1310. The actuator lever 1310 may ride along a top surface of the rack 238. According to various embodiments, the rack 238 may define an indentation 1312 along its top surface. The indentation 1312 may be positioned longitudinally on the rack such that the actuator lever 1310 of the switch 1220 falls into the indentation 1312 at the predetermined position of the firing stroke referred to with respect to FIG. 54. Alternatively, it will be appreciated that the rack 238 may comprise a protrusion positioned to contact the actuator at the predetermined part of the firing stroke.

FIG. 59 illustrates another cut away view of one embodiment of the instrument 102 showing the end-of-stroke/motor reverse switch 1204. The switch 1204 may comprise an actuator 1322. The actuator 1322 may be activated by an external reverse motor button 1320 or by the rack 238 as it reaches the distal end of its travel (e.g., indicating an end of the stroke of the firing bar 108). For example, the rack 238 may comprise a protrusion 1324 that contacts the actuator 1322 of the switch 1204. Also, for example, the rack 238 may comprise an indentation or cavity (not shown) positioned to contact the actuator 1322 at the distal end of the travel of the track 238.

Although the device described herein shows the rotational movement of the motor 222 being translated into longitudinal motion in the handle 106 (e.g., via the rack 238 and firing bar 108), it will be appreciated that instruments according to various embodiments may perform this translation outside of the handle, for example, in the shaft, or at the end effector itself. For example, in some embodiments, a rotating drive shaft (not shown) may extend some or all of the way through the shaft 114 from the handle 106 to the end effector 104. The various switches described herein may be utilized in such an embodiment. For example, the various switches described herein may be positioned to be actuated in the same relationship to the position of the firing bar 108 as described herein.

While the present invention has been illustrated by description of several embodiments and while the illustrative embodiments have been described in considerable detail, it is not the intention of the applicant to restrict or in any way limit the scope of the appended claims to such detail. Additional advantages and modifications may readily appear to those skilled in the art. For another example, although the E-beam firing beam 108 has advantages for an endoscopically employed surgical severing and stapling instrument 102, a similar E-Beam may be used in other clinical procedures. It is generally accepted that endoscopic procedures are more common than laparoscopic procedures. Accordingly, the present invention has been discussed in terms of endoscopic procedures and apparatus. However, use herein of terms such as "endoscopic", should not be construed to limit the present invention to a surgical stapling and severing instrument for use only in conjunction with an endoscopic tube (i.e., trocar). On the contrary, it is believed that the present invention may find use in any procedure where access is limited to a small incision, including but not limited to laparoscopic procedures, as well as open procedures. For yet another example, although an illustrative handle portion 106 described herein is manually operated by a clinician, it is consistent with aspects

22

of the invention for some or all of the functions of a handle portion to be powered (e.g., pneumatic, hydraulic, electromechanical, ultrasonic, etc.). Furthermore, controls of each of these functions may be manually presented on a handle portion or be remotely controlled (e.g., wireless remote, automated remote console, etc.).

It is to be understood that at least some of the figures and descriptions herein have been simplified to illustrate elements that are relevant for a clear understanding of the disclosure, while eliminating, for purposes of clarity, other elements. Those of ordinary skill in the art will recognize, however, that these and other elements may be desirable. However, because such elements are well known in the art, and because they do not facilitate a better understanding of the disclosure, a discussion of such elements is not provided herein.

While several embodiments have been described, it should be apparent, however, that various modifications, alterations and adaptations to those embodiments may occur to persons skilled in the art with the attainment of some or all of the advantages of the disclosure. For example, according to various embodiments, a single component may be replaced by multiple components, and multiple components may be replaced by a single component, to perform a given function or functions. This application is therefore intended to cover all such modifications, alterations and adaptations without departing from the scope and spirit of the disclosure as defined by the appended claims.

Any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated materials does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

What is claimed is:

1. A powered surgical instrument for cutting and fastening tissue, the instrument comprising:

an end effector comprising:

a first jaw member;

a second jaw member coupled to move relative to the first jaw member from an open position, where the jaw members are apart from one another, to a closed position; and

a firing bar positioned to fire by translating within the end effector when the first and second jaw members are in the closed position;

a drive device mechanically coupled to the firing bar;

a drive train mechanically coupled to the drive device and to the firing bar;

a clamping trigger mechanically coupled to the end effector such that the clamping trigger defines an actuated position that causes the second jaw member to pivot towards the first jaw member and an un-actuated position that causes the second jaw member to pivot away from the first jaw member;

a control circuit, wherein the control circuit comprises:

a power supply comprising a first terminal and a second terminal;

a switching device alternately configurable between a first connection state and a second connection state;

23

a firing switch positioned on a first electrical connection between the power supply, the drive device, and the switching device, wherein the firing switch defines an actuated position;

a clamp switch in mechanical communication with the clamping trigger and positioned on a second electrical connection between the power supply and the switching device;

an end-of-stroke switch defining a first position in which the end-of-stroke switch forms part of a third electrical connection between the first terminal of the power supply and the drive device, and a second position in which the end-of-stroke switch forms part of a fourth electrical connection between the second terminal of the power supply, the switching device, and the drive device, wherein the end-of-stroke switch is in physical contact with at least a portion of the drive train positioned to transition the end-of-stroke switch to the second position when the firing bar reaches an end of stroke;

wherein the first electrical connection is completed when the firing switch is in the actuated position and the switching device is in the first connection state;

wherein, upon the end-of-stroke switch transitioning to the second position, the fourth electrical connection is completed, causing the switching device to transition to the second state, wherein the transition to the second state causes the switching device to break the first electrical connection; and

wherein, when the clamping trigger is in the un-actuated position, the clamp switch is closed to complete the second electrical connection causing the switching device to transition to the first state.

2. The surgical instrument of claim 1, wherein the first jaw member is shaped to receive a staple cartridge and the second jaw member defines at least one staple pocket for receiving and forming a staple.

3. The surgical instrument of claim 2, wherein the firing bar is in mechanical communication with a staple driver to push the staple driver distally upon firing.

4. The surgical instrument of claim 1, wherein the firing bar comprises a cutting edge.

5. The surgical instrument of claim 1, wherein the drive train comprises a rack translatable distally and proximally, wherein the rack is in mechanical communication with the firing bar, wherein the rack defines at least one geared face.

6. The surgical instrument of claim 5, wherein the drive device is positioned to rotate a gear in mechanical communication with the rack.

7. The surgical instrument of claim 6, wherein rotational motion of the drive device and gear in a first direction causes the rack and the firing bar to translate distally, and wherein rotational motion of the drive device and gear in a second direction causes the rack and the firing bar to translate proximally.

8. The surgical instrument of claim 5, wherein the rack defines a protrusion, and wherein the end-of-stroke switch comprises an actuator positioned to contact the protrusion to actuate the end-of-stroke switch when the rack reaches a position indicating the end of the firing bar stroke.

9. The surgical instrument of claim 5, wherein the control circuit further comprises a stroke position switch positioned to actuate when the firing bar reaches a predetermined position; and a resistive element in electrical communication with the stroke position switch, wherein the stroke position switch is electrically connected to electrically switch the resistive

24

element between the power supply and the drive device until actuated in response to the firing bar reaching the predetermined position.

10. The surgical instrument of claim 9, wherein the stroke position switch comprises an actuator, and wherein the rack defines a cavity positioned to receive the actuator of the stroke position switch to actuate the stroke position switch when the firing bar reaches the predetermined position.

11. The surgical instrument of claim 1, wherein the instrument further comprises a clamp lock mechanically positioned to lock the second jaw member against the first jaw member.

12. The surgical instrument of claim 11, wherein the clamp switch comprises an actuator positioned to be actuated upon release of the clamp lock.

13. The surgical instrument of claim 1, wherein the control circuit further comprises an emergency access door switch coupled to an emergency access door of the instrument such that opening of the emergency access door actuates the emergency access door switch to break an electrical connection to the power supply.

14. The surgical instrument of claim 1, wherein the switching device is a relay.

15. The surgical instrument of claim 14, wherein the relay is a latching relay.

16. The surgical instrument of claim 1, wherein the relay is at least one of a mechanical relay and an electromagnetic relay.

17. A powered surgical instrument for cutting and fastening tissue, the instrument comprising:

an end effector comprising:

a first jaw member;

a second jaw member coupled to move relative to the first jaw member from an open position, where the jaw members are apart from one another, to a closed position; and

a firing bar positioned to fire by translating within the end effector when the first and second jaw members are in the closed position; and

a drive device mechanically coupled to the firing bar; and a clamping trigger mechanically coupled to the end effector such that actuation of the clamping trigger causes the second jaw member to pivot towards the first jaw member;

a rack defining a protrusion, wherein the rack is translatable distally and proximally, wherein the rack is in mechanical communication with the firing bar, and wherein the rack defines at least one geared face;

a control circuit, wherein the control circuit comprises:

a firing switch configured to be in electrical communication with a power supply for powering the drive device and in electrical communication with the drive device;

a clamp switch in mechanical communication with the clamping trigger;

a latching device in electrical communication with the clamp switch, the power supply and the drive device; and

an end-of-stroke switch in electrical communication with the latching device, wherein the end-of-stroke switch comprises an actuator positioned to contact the protrusion of the rack to actuate the end-of-stroke switch when the rack reaches a position indicating the end of the firing bar stroke; and

wherein the firing switch is electrically connected to, upon actuation, connect the power supply to the drive device via a first connection comprising the latching device and the firing switch;

25

wherein the end-of-stroke switch is electrically connected to, upon actuation, cause a change in a state of the latching device to break the first connection between the power supply and the drive device.

18. A powered surgical instrument for cutting and fastening tissue, the instrument comprising:
- an end effector comprising:
 - a first jaw member;
 - a second jaw member coupled to move relative to the first jaw member from an open position, where the jaw members are apart from one another, to a closed position; and
 - a firing bar positioned to fire by translating within the end effector when the first and second jaw members are in the closed position; and
 - a drive device mechanically coupled to the firing bar; and
 - a clamping trigger mechanically coupled to the end effector such that actuation of the clamping trigger causes the second jaw member to pivot towards the first jaw member;
 - a rack translatable distally and proximally, wherein the rack is in mechanical communication with the firing bar, and wherein the rack defines at least one geared face;
 - a control circuit, wherein the control circuit comprises:
 - a firing switch configured to be in electrical communication with a power supply for powering the drive device and in electrical communication with the drive device;
 - a clamp switch in mechanical communication with the clamping trigger;
 - a latching device in electrical communication with the clamp switch, the power supply and the drive device; and
 - an end-of-stroke switch in electrical communication with the latching device;
 - a stroke position switch positioned to actuate when the firing bar reaches a predetermined position; and
 - a resistive element in electrical communication with the stroke position switch;
 - wherein the firing switch is electrically connected to, upon actuation, connect the power supply to the drive device via a first connection comprising the latching device and the firing switch;
 - wherein the end-of-stroke switch is positioned to be actuated at an end of stroke of the firing bar and, upon actuation, cause a change in a state of the latching device to break the first connection between the power supply and the drive device;
 - wherein the stroke position switch is electrically connected to electrically switch the resistive element between the

26

power supply and the drive device until actuated in response to the firing bar reaching the predetermined position;

wherein the stroke position switch comprises an actuator, and wherein the rack defines a cavity positioned to receive the actuator of the stroke position switch to actuate the stroke position switch when the firing bar reaches the predetermined position.

19. A powered surgical instrument for cutting and fastening tissue, the instrument comprising:
- an end effector comprising:
 - a first jaw member;
 - a second jaw member coupled to move relative to the first jaw member from an open position, where the jaw members are apart from one another, to a closed position; and
 - a firing bar positioned to fire by translating within the end effector when the first and second jaw members are in the closed position; and
 - a drive device mechanically coupled to the firing bar; and
 - a clamping trigger mechanically coupled to the end effector such that actuation of the clamping trigger causes the second jaw member to pivot towards the first jaw member;
 - an emergency access door; and
 - a control circuit, wherein the control circuit comprises:
 - a firing switch configured to be in electrical communication with a power supply for powering the drive device and in electrical communication with the drive device;
 - a clamp switch in mechanical communication with the clamping trigger;
 - a latching device in electrical communication with the clamp switch, the power supply and the drive device; and
 - an end-of-stroke switch in electrical communication with the latching device;
 - an emergency access door switch coupled to the emergency access door such that opening of the emergency access door actuates the emergency access door switch to break an electrical connection to the power supply; and
 - wherein the firing switch is electrically connected to, upon actuation, connect the power supply to the drive device via a first connection comprising the latching device and the firing switch;
 - wherein the end-of-stroke switch is positioned to be actuated at an end of stroke of the firing bar and, upon actuation, causes a change in a state of the latching device to break the first connection between the power supply and the drive device.

* * * * *